Instruction Manual

FLUKE

ELECTRONICS FOR INDUSTRY
INSTRUMENTS / COMPONENTS

JOHN FLUKE MFG. CO. INC.
P. O. Box 7428 Seattle 33, Washington

October 25, 1961

MODEL 803
AC/DC
DIFFERENTIAL VOLTMETER

803_____

803R_____

© COPYRIGHT, JOHN FLUKE MFG. CO., INC., 1970

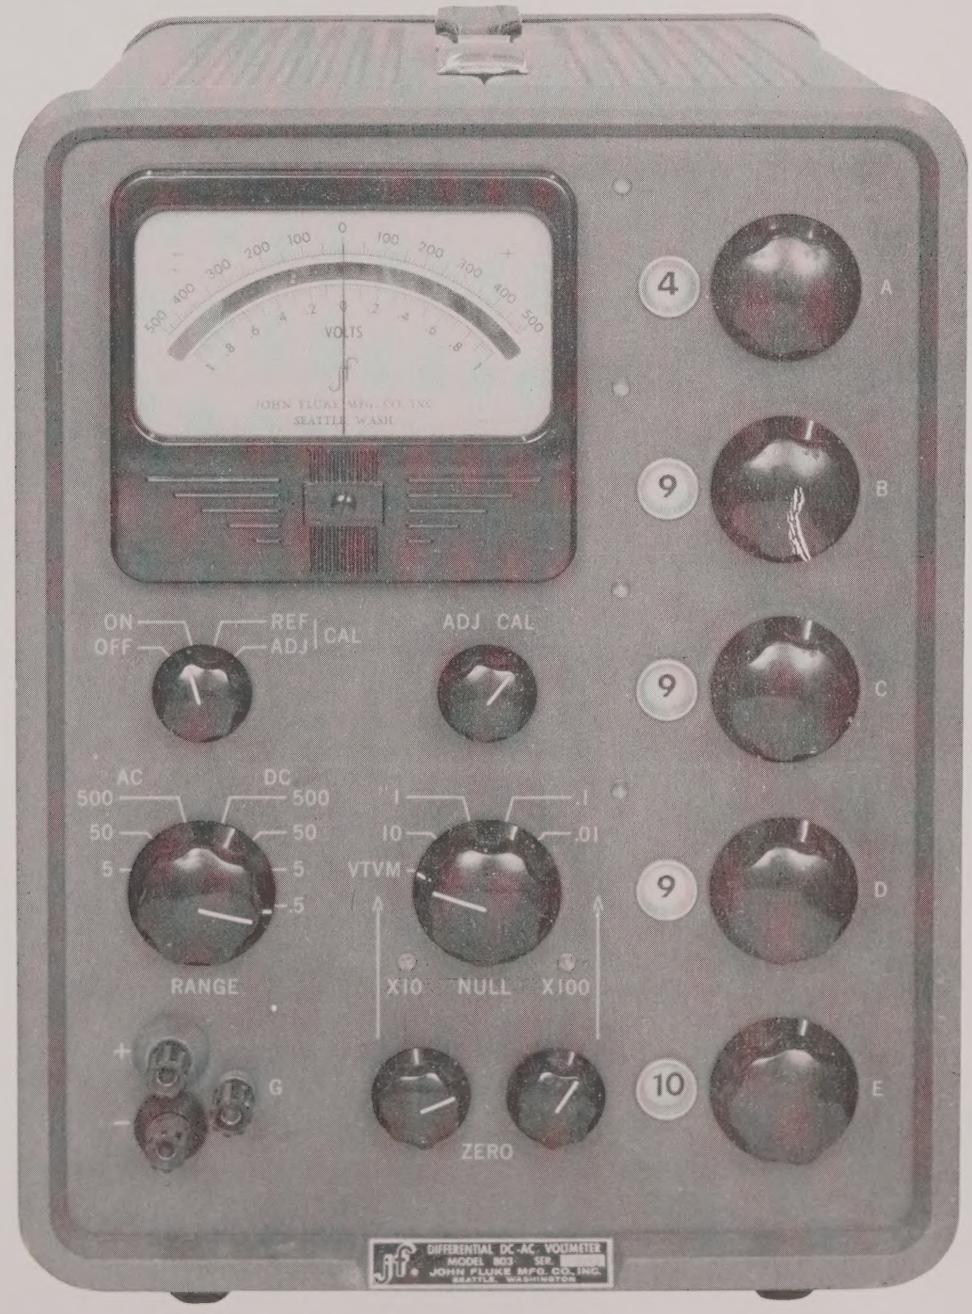
VOLTS
JOHN FLUKE MFG. CO. INC.
SEATTLE, WASH.
ON
OFF
REF
ADJ
CAL
ADJ CAL
AC
DC
500
50
5
.5
RANGE
I
.1
10
.01
VTVM
X10
NULL
X100
ZERO
+
−
G
4
A
9
B
9
C
9
D
10
E
DIFFERENTIAL DC-AC VOLTMETER
MODEL 803 SER.
JOHN FLUKE MFG. CO. INC.
SEATTLE, WASHINGTON

MODEL 803

TABLE OF CONTENTS

Section	Title	Page
I	INTRODUCTION AND SPECIFICATIONS	1-1
	1-1. General	1-1
	1-2. Specifications	1-1
II	OPERATING INSTRUCTIONS	2-1
	2-1. Controls and Terminals	2-1
	2-2. Preliminary Operation	2-1
	2-3. Measurement of DC Voltage	2-1
	2-4. Measurement of AC Voltage	2-2
	2-5. Measurement of Voltage Excursions About a Nominal Value	2-2
	2-6. Use as a Conventional VTVM	2-2
	2-7. Measurement of High Resistance	2-2
	2-8. Use of the 803 With a Recorder	2-2
	2-9. Notes on Measuring AC and DC Voltages	2-3
III	THEORY OF OPERATION	3-1
	3-1. General	3-1
	3-2. 500 V DC Reference Power Supply	3-1
	3-3. Kelvin-Varley Divider	3-1
	3-4. Vacuum Tube Voltmeter (VTVM)	3-1
	3-5. Chopper-Amplifier	3-2
	3-6. Converter	3-2
	3-7. Converter Power Supply	3-2
IV	MAINTENANCE	4-1
	4-1. General	4-1
	4-2. Preventive Maintenance	4-1
	4-3. Troubleshooting	4-1
	4-4. Calibration	4-4
V	LIST OF REPLACEABLE PARTS	5-1
	WARRANTY	
	CIRCUIT DIAGRAM	

Digitized by the Internet Archive
in 2025

https://archive.org/details/manualsplus_08607

SECTION I

INTRODUCTION AND SPECIFICATIONS

1-1. GENERAL

a. The Model 803 AC-DC Differential Voltmeter has enjoyed wide acceptance in the field of voltage measurements. The high accuracy, portability, and compactness of the 803 make this instrument ideal for almost any application. Ease of operation and high reliability contribute to the outstanding performance which makes the 803 a universally accepted instrument.

b. The heart of the 803 is a precision 500 V DC reference power supply. This 500 volts can be precisely divided into increments as small as 10 microvolts by means of five voltage dials. Unknown AC or DC voltages are matched against the precise internal voltage until no deflection occurs on the panel meter. The unknown voltage is then simply read from the voltage dials. In the highest null sensitivity range, potential differences between unknown and reference voltage as small as 0.01 volts will cause full scale meter deflection.

c. At null, the 803 presents an infinite input impedance to the voltage under measurement, thereby completely eliminating circuit loading.

d. The instrument may also be used as a conventional VTVM or as a megohmmeter.

e. The Model 803 has been thoroughly checked and tested prior to shipment, and is ready for immediate use. Upon receipt, inspect carefully for any damage that may have occurred in transit. Refer to the warranty page at the back of this manual if shipping damage is evident.

1-2. SPECIFICATIONS

Following are the specifications of the Model 803.

Input Voltage Range	Recommended Null Range	Input Impedance At Null
DC:		
50-500	10-0-10	Infinite
	1-0-1	"
5-50	1-0-1	"
	0.1-0-0.1	"
0.5-5	0.1-0-0.1	"
	0.01-0-0.01	"
0-0.5	0.1-0-0.1	"
	0.01-0-0.01	"
AC:		
50-500	10-0-10	1M, 25 uuf
	1-0-1	"
5-50	1-0-1	"
	0.1-0-0.1	"
.05-5	0.1-0-0.1	"
	0.01-0-0.01	"

Resolution:

Input Voltage Range	Dial Resolution (Volts)	Meter Resolution (Volts)
DC:		
50-500	0.01	0.005
5-50	0.001	0.0005
0.5-5	0.0001	0.00005
0-0.5	0.00001	0.00005
AC:		
50-500	0.01	0.005
5-50	0.001	0.0005
0.05-5	0.0001	0.00005

Accuracy:

DC: ±0.05% of input voltage from 0.1 to 500 V
±0.1% of input voltage or 0.00005 V, whichever is greater from 0 to 0.1 V.

AC: ±0.2% of input voltage from 0.5 to 500 V, reduced accuracy from 0.05 to 0.5 V.

VACUUM TUBE VOLTMETER

Voltage Ranges:

	Input Voltage Range	Input Impedance
DC:	±500	10M
	±50	10M
	±5	10M
	±0.5	10M
	±10*	10M
	±1 *	10M
	±0.1*	1M
	±0.01*	1M
AC:	0-500	1M, 25 uuf
	0-50	"
	0-5	"
	0-100*	"
	0-10*	"
	0-0.1*	"
	0-0.01*	"

*Using Null Ranges.

Accuracy: ±4%.

GENERAL SPECIFICATIONS

Reference Stability:
±0.01% maximum for 105 to 130 VAC line.
±0.01% per hour after 30 minute warmup.

AC to DC Converter Frequency Response:
30 CPS to 10 KC.

Input Power:
175 watts at 117/234 volts, 50/60 cycles.

Size:
Cabinet Model - 13" H x 9-3/4" W x 16" D.
Rack Model - 8-3/4" H x 19" W x 17-5/16" D.

Weight:
Cabinet Model - 30 pounds.
Rack Model - 38 pounds.

SECTION II
OPERATING INSTRUCTIONS

2-1. CONTROLS AND TERMINALS

The functions of the operating controls and terminals of the Model 803 are listed below:

a. The OFF-ON-CAL switch controls AC line power on cabinet model instruments. When placed in the CAL REF position, the chopper amplifier output may be calibrated, and in the CAL ADJ position, the internal 500 V DC reference voltage is calibrated. On rack model instruments, this switch is labelled OPERATE-CAL and line power is controlled by a toggle switch.

b. The RANGE switch selects AC voltage ranges of 500, 50, and 5 volts, or DC ranges of 500, 50, 5, and 0.5 volts.

c. The NULL switch is placed in the VTVM position to determine the approximate value of the unknown voltage prior to any differential measurements. The four null voltage ranges of 10, 1, 0.1, and 0.01 volts are used when differential measurements are made. For DC measurements, these ranges represent full scale differences between the unknown voltage and the portion of internal 500 V DC that is dialed up on the five voltage dials. For AC measurements, the null sensitivities are reduced on the 500 VAC and 50 VAC ranges as indicated by the X100 and X10 null range multiplier adjacent to the NULL switch. For example, on the 500 VAC range position, the X100 null multiplier lamp would light, and the maximum full scale voltage difference between internal reference and unknown would be 100 multiplied by the 0.01V null range, or 1 volt.

d. A, B, C, D, and E voltage dial settings provide an in-line readout of the amount of internal 500 V DC necessary to null (match) the unknown. Illuminated decimal points adjacent to the voltage dials change as the range of the instrument is changed.

e. ZERO controls are provided for calibrating the VTVM-10V-1V null ranges and the 0.1V-0.01V null ranges.

f. The positive input binding post is isolated from the chassis of the instrument, and the negative post is shunted to the chassis with a 1 UFD capacitor. Either post may be grounded or both may be "floated" from ground; however, since the instrument is equipped with 3-wire line cord with the third wire fastened to the chassis, the external circuit should be checked to avoid conflicts in grounding.

g. The ADJ CAL potentiometer controls calibration of the 500 V DC reference supply when the ON-OFF-CAL switch is in CAL ADJ position.

2-2. PRELIMINARY OPERATION

The following procedure prepares the 803 for operation.

a. Connect the power plug to an AC power source. The instrument is wired to operate on 117 VAC. Note on the schematic diagram that 220 VAC or 234 VAC operation is possible by rewiring the primary of the power transformer, and substituting a 1.5 Amp. line fuse.

b. Turn the RANGE switch to the 500 V DC position.

c. Turn the NULL switch to the VTVM position.

d. Turn all voltage dials to zero.

e. Place the instrument in operation by turning the OFF-ON-CAL control to ON. On rack models, turn the line power toggle switch to ON. The decimal lamp will light, indicating power is applied.

f. Allow a warmup period of at least ten minutes.

g. Adjust the VTVM-10V-1V ZERO control for zero meter deflection.

h. Turn the OFF-ON-CAL switch (OPERATE-CAL on rack models) to the CAL REF position and adjust the 0.1V-0.01V ZERO control for zero meter deflection.

i. Advance the switch against spring tension to the CAL ADJ position, and calibrate the internal 500 V DC reference supply by zeroing the meter with the ADJ CAL control.

j. Return the switch to the ON position (OPERATE position on rack models). The instrument is ready for use.

CAUTION

For personnel safety, the instrument is equipped with a 3-wire line cord so that the chassis will be grounded. Do not connect either binding post to the chassis ground post unless the circuit under test has been checked for conflicts in grounding.

2-3. MEASUREMENT OF DC VOLTAGE

a. After completing preliminary operation, connect the unknown voltage to the input binding posts with the range switch in the 500 V DC position. With the NULL switch in the VTVM position, the approximate value of the unknown will be indicated on the top meter scale. If the meter reads to the left, the polarity of the unknown voltage is opposite to the polarity of the instrument input, and the connections should be reversed.

b. Turn the RANGE switch to the lowest DC range which will give an on-scale reading and observe the approximate value of the unknown voltage.

c. Observe the position of the decimal light, and set the five voltage dials to the approximate voltage determined in step b. For example, if the approximate voltage is 3.5 volts, turn the A dial to 3, B dial to 5, and C, D, and E dials to zero.

d. Turn the NULL switch to the 10V position and adjust the voltage dials for zero meter deflection.

e. Turn the NULL switch to the 1V, 0.1V, and 0.01V positions, adjusting the voltage dials for zero meter deflection in each position.

f. Read the unknown voltage directly from the five voltage dials.

2-4. MEASUREMENT OF AC VOLTAGES

a. After completing preliminary operation, place the RANGE switch in the 500 VAC position.

b. Connect the unknown AC voltage to the positive and negative binding posts.

c. Proceed in the same manner as in measurement of DC voltage, step b and on.

2-5. MEASUREMENT OF VOLTAGE EXCURSIONS ABOUT A NOMINAL VALUE

a. After completing preliminary operation, set up the nominal voltage on the five voltage dials.

b. Turn the RANGE switch to the correct AC or DC position.

c. Connect the voltage under measurement to the input binding posts.

d. Turn the NULL switch to the position which allows the voltage excursions to remain on-scale. The NULL switch settings indicate full scale right and left meter deflections, except when the RANGE switch is set in the 500 VAC or 50 VAC positions. In these cases, the full scale excursions are equal to the NULL range setting multiplied by the X100 or X10 factor indicated by the NULL multiplier lamps.

2-6. USE AS A CONVENTIONAL VTVM

If it is desired to use the instrument as a VTVM only, the NULL ranges may be converted to VTVM ranges by setting the voltage dials to zero. Proceed as follows:

a. Perform preliminary operation procedures stated in paragraph 2-2.

b. Consult figure 2-1 and select full scale voltage deflection desired. If the approximate value of the voltage to be measured is unknown, select the 500V range initially.

c. Set RANGE switch, NULL switch, and voltage dials as indicated for the range selected.

d. Connect the voltage to be measured to the input binding posts. Deflection to the right indicates same polarity as binding posts.

e. Read voltage from upper or lower scale as listed in figure 2-2.

2-7. MEASUREMENT OF HIGH RESISTANCES

One of the important features of the Model 803 is the ability to be used as a megohmmeter for high resistance measurements from 1 to 500,000 megohms. In this application, connect the minus input terminal to the chassis ground post and use short isolated leads to the unknown resistance to prevent measuring leakage resistance of the leads. Proceed as follows:

a. Perform the preliminary operation procedure. For resistances over a range from 1 to 500 megohms, set RANGE switch to 500 V DC, NULL switch to 10V, and adjust voltage dials for full scale deflection with the unknown resistance connected to the input terminals. Subtract 10.00 from the dial reading for the resistance of the unknown in megohms.

b. For resistances over a range from 500 to 5000 megohms, set RANGE switch to 500 V DC, NULL switch to 1V, and adjust voltage dials for full scale meter deflection. Subtract 1.00 from the dial reading and multiply the result by 10 for the resistance of the unknown in megohms.

c. Between 5000 and 500,000 megohms, the resistance is calculated from the following formula:

$$R_X = 10 \left(\frac{E}{E_m} - 1\right), \text{ where}$$

R_X = unknown resistance in megohms
E = voltage indicated by voltage dials
E_m = meter reading from 0 to 1V on the bottom meter scale (1V null range)
10 = megohms input resistance of the VTVM circuit in the 1V null range

Set the RANGE switch to 500 V DC, NULL switch to the 1V range, and adjust the voltage dials for a convenient meter deflection. Substitute the meter reading in volts and the voltage dial setting in volts into the equation to obtain unknown resistance.

2-8. USE OF THE 803 WITH A RECORDER

Recorder output binding posts and level control are provided on the rear of the 803 for monitoring the excursions of an unknown voltage from the voltage indicated by the dial settings. The leakage resistance between the recorder and ground must be greater than 500,000 megohms or the accuracy of the 803 will be impaired. The John Fluke Model A-70 Potentiometric Recorder (manufactured by the Texas Instrument Co.) is recommended for this application. Set up the recorder as follows:

a. Connect recorder input terminals to 803 output terminals with teflon leads.

CAUTION

Do not ground either of the recorder output terminals to the chassis of the 803. It is possible that the 1/200 ampere fuse at the output of the Kelvin-Varley divider will be blown.

b. After connecting the recorder, perform preliminary operation.

c. Check for excessive leakage by connecting a standard cell to the 803 and measuring the EMF. Then alternately connect and disconnect the recorder leads at the rear of the 803. More than 1/4 small scale division deflection of the 803 indicates excessive leakage has been introduced by the recorder, and 803 accuracy will be impaired. If less than 1/4 division, make another check by setting the RANGE switch to 500 V DC, NULL switch to 1V, and all voltage dials to zero. Zero the instrument with the VTVM-10V-1V control, then set the voltage dials to 400.00. A properly operating 803 will deflect less than 1/4 small scale division with the recorder leads disconnected. If more than 1/4 division deflection occurs with leads connected, accuracy will be impaired.

d. When leakage checks have been completed, short the input terminals of the 803.

e. Turn the RANGE switch to the 50V position, NULL switch to the 10V position, and dial up 10.000 volts. The meter will deflect full scale, giving a maximum output at the recorder terminals of 15 millivolts.

f. Turn the GAIN ADJ potentiometer adjacent to the recorder terminals for the recorder deflection that is desired to correspond to full-scale 803 deflection.

g. Remove the short from the 803 input terminals. The 803-Recorder combination is ready for use. Proceed as instructed under paragraph 2-5.

2-9. NOTES ON MEASURING AC AND DC VOLTAGES

a. When selecting the AC or DC range of operation, always use the lowest range that will give an on-scale reading with the NULL switch in the VTVM position. This will assure that the maximum number of Kelvin-Varley voltage dials will be used, providing the best accuracy. For example, when measuring 3.52 volts, set the RANGE switch to the 5 V DC position and use all 5 voltage dials, rather than the 500 V DC position, where only three dials could be used.

b. Any NULL range may be used at any input voltage. However, it is recommended that the 10V and 1V null ranges be used for voltages higher than 50 volts; 10V, 1V, and 0.1V null ranges are recommended between 5 and 50 volts. A badly fluctuating line voltage or an unstable input voltage may cause meter rattle or erratic movements if higher null sensitivities are used on these voltage ranges.

c. AC components do not normally effect DC measurements in the 10V and 1V null ranges. In the 0.1V and 0.01V null ranges, the filter network at the input of the chopper-amplifier will attenuate the AC component. This filter has an attenuation ratio of 330 to 1 at 60 cycles. For example, a one-half volt, 60 cycle AC component will be reduced to slightly over one millivolt. If large AC components are present on the DC to be measured, and the 0.1V and 0.01V (chopper-amplifier) null ranges must be used, additional filtering is required. If the AC is of a single frequency, a twin-T filter is effective and has the advantage of low total series resistance. If the AC is of variable frequency, an ordinary low-pass filter may be used. In either case, the capacitors used should be high quality units of high leakage resistance.

d. When making measurements of negative DC voltage, the positive binding post should not be connected to the chassis binding post. This would place C101, a 1 MFD capacitor, directly across the input. Since the chassis binding post is connected to earth ground through the 3-wire line cord, this may happen inadvertantly if the source of the voltage being measured has the positive side grounded. When C101 is directly across the voltage being measured, a small 60 cycle signal (50 millivolts or less) appears across this capacitor due to slightly unbalanced capacitances between the power transformer high voltage windings and the core. This may affect the true DC reading, or the source under measurement, or both.

e. When making AC measurements, the presence of harmonics may have an effect on accuracy. Figure 2-2 indicates how accuracy will be affected by various harmonics for different percentages of distortion.

Full-Scale Deflection	Range Switch	Null Switch	Multiplier	Voltage Dials	Meter Scale
DC					
500-0-500	500 V DC	VTVM	-	No effect	Upper
50-0-50	50 V DC	VTVM	-	No effect	Upper
10-0-10	No effect	10	-	All zero	Lower
5-0-5	5 V DC	VTVM	-	No effect	Upper
1-0-1	No effect	1	-	All zero	Lower
0.5-0-0.5	0.5 V DC	VTVM	-	No effect	Upper
0.1-0-0.1	No effect	0.1	-	All zero	Lower
0.01-0-0.01	No effect	0.01	-	All zero	Lower
AC					
500-0-500	500 VAC	VTVM	-	No effect	Upper
100-0-100	500 VAC	1	X100	All zero	Lower
50-0-50	50 VAC	VTVM	-	No effect	Upper
10-0-10	50 VAC	1	X10	All zero	Lower
5-0-5	5 VAC	VTVM	-	No effect	Upper
1-0-1	5 VAC	1	-	All zero	Lower
0.1-0-0.1	5 VAC	0.1	-	All zero	Lower
0.01-0-0.01	5 VAC	0.01	-	All zero	Lower

Figure 2-1. VTVM RANGES

HARMONIC	% DISTORTION	%ERROR* MAXIMUM POSITIVE	MAXIMUM NEGATIVE
Any even harmonic	0.1	0.000	
	0.5	0.0001	
	1.0	0.005	
	2.0	0.020	
Third harmonic	0.1	0.033	0.033
	0.5	0.168	0.167
	1.0	0.338	0.328
	2.0	0.687	0.667
Fifth harmonic	0.1	0.020	0.020
	0.5	0.101	0.099
	1.0	0.205	0.195
	2.0	0.420	0.380

*Error depends upon phase relationship between harmonic and fundamental for odd harmonics, i.e. error can be any value between maximum positive and maximum negative, including zero.

Figure 2-2. HARMONIC DISTORTION

SECTION III
THEORY OF OPERATION

3-1. GENERAL

a. A functional schematic of the Model 803 is shown following Section V. The functional method of circuit representation is designed to aid the reader in discussions of circuit theory and troubleshooting.

b. As seen on the schematic, the principle circuit divisions are: 500 V DC reference power supply; Kelvin-Varley divider; vacuum tube voltmeter (VTVM); chopper-amplifier; converter, and converter power supply.

3-2. 500 V DC REFERENCE POWER SUPPLY

a. When the 803 is used in the differential mode for voltage measurements, an internal precision DC voltage is nulled or matched against the unknown voltage. An extremely accurate reference voltage is therefore required. This voltage is developed by the 500 V DC reference supply, V1 through V8.

b. V1, (full wave rectifier) and the associated filter network, supply raw DC voltage at approximately 1000 volts to the pre-regulator tube V2. Any change in the output of the pre-regulator is felt at the grid of V3, the cathode of which is clamped by voltage regulator V4. The plate potential of V3, which is coupled to the grid of V2, will change to correct the output of the pre-regulator, which should be approximately 650 volts to V5A, the main regulator.

c. The grid of the main regulator is driven by V5B, which in turn is driven by differential amplifier V8. Changes in the output of the main regulator are felt at pin 2 (grid) of V8. Since the opposite grid (pin 7) is clamped by voltage regulators V6 and V7, and the cathodes are tied together, V8 drives the grid and cathode of V5B in opposite directions to change the grid potential of V5A, correcting the main regulator output. The output is maintained at 500 V DC ±0.01%.

d. In the 500 V DC position, the RANGE switch (S102E) passes this 500 volts directly to the Kelvin-Varley divider. In the 50 V DC, 5 V DC, and 0.5 V DC positions, range resistors controlled by S102F divide the reference voltage to 50 V DC, 5 V DC, and 0.5 V DC respectively. In all AC positions of the RANGE switch, only 5 volts of the reference supply is used, due to the fact that the maximum output of the AC to DC converter is 5 volts. This is explained in the discussion of the converter.

3-3. KELVIN-VARLEY DIVIDER

a. Each one of the four precision voltages available from the reference supply must be made adjustable through a precision divider string so that unknown voltages may be nulled or matched exactly. The five Kelvin-Varley decade resistor strings accomplish this function.

b. Note that each string, with the exception of the first, parallels two resistors of the string that preceeds it. Between the two wipers of S104 (voltage dial "A") then, there is a total resistance of 40K and a total voltage of 100 V DC, with the RANGE switch in the 500 V DC position. Across the wipers of S105, S106, and S107, there are 10 V DC, 1 V DC, and 0.1 V DC respectively. S108 (dial "E") picks increments of 0.01 V DC from the last decade. These voltages are reduced by a factor of 10 for each lower range voltage.

c. All resistors of each decade are matched and all decades are matched for each instrument, providing an over-all divider accuracy of 0.005%.

d. With the NULL switch in any null range, the output of the Kelvin-Varley divider appears at the grid of one-half of the VTVM differential amplifier, V204B. A 1/200 ampere (5 milliampere) fuse protects this output.

3-4. VACUUM TUBE VOLTMETER (VTVM)

a. When operating in the differential mode, Kelvin-Varley output voltage appears on the grid of V204B, one-half of differential amplifier V204. The unknown voltage appears on the grid of V204A, the other half of the differential amplifier. Any difference between these potentials will be indicated by the meter which is coupled between the cathodes of V204. When the Kelvin-Varley output voltage exactly matches the unknown, the meter will read zero and no current will be drawn from the source being measured, because the same potential exists on both sides of the input resistances R105 through R109.

b. An 0.5 volt difference between potentials on the grids of the differential amplifier will drive the meter to full-scale deflection. As seen on the schematic, the voltage division across R105, R106, and R107 will provide 0.5 volt difference to the differential amplifier grids in the 10V null range if the actual difference between unknown and Kelvin-Varley voltage is 10 volts; in the 1V null range, a different division of potential will pro-

vide 0.5 volt to V204 for a 1V difference between unknown voltage and reference voltage.

c. In the 0.1V and 0.01V null ranges, the chopper-amplifier is used to provide the 0.5 volts necessary for full-scale deflection of voltage differences as small as 0.1 and 0.01 volt.

d. When used as a conventional VTVM, the grid of V204B is connected to the 0 volt buss, or negative binding post. With the range switch in the 0.5 V DC position, the 0 to 0.5 V DC unknown voltage appears directly on the grid of V204A, and will indicate the approximate value of the unknown. Input divider resistors R110 through R116 maintain the 0 to 0.5 grid voltage range for all instrument voltage ranges. The input resistance of the instrument in the VTVM position is seen to be 10 megohms, the sum of R110, R112, R114, and R116.

c. The chopper-amplifier is used during calibration of the 500 V DC reference supply. With the OFF-ON-CAL switch in the CAL ADJ position, a fixed percentage of the reference supply is compared to the precise EMF of the internal standard cell. Any difference in potential is fed to the chopper-amplifier and VTVM so that the reference supply may be adjusted by means of R119 (ADJ CAL potentiometer) to 500 V DC ±0.01%.

3-5. CHOPPER-AMPLIFIER

a. Since the grid drive to V204 must be 0.5 volts for full-scale meter deflection, a chopper amplifier is employed to boost the DC potential difference between the unknown and internal reference, when operating in the 0.1V and 0.01V null ranges.

b. The chopper-amplifier is a fixed-gain device consisting of V205 and V206. A 60 cycle chopper modulates any DC level appearing at the input. The resulting square-wave is amplified and demodulated by another chopper contact. The resulting DC gain is approximately 50. Therefore, for 0.01 volts maximum input, the output will be 0.5 volts, enough for full-scale deflection of the VTVM. In the 0.1V null range, the input to the chopper amplifier is still 0.01 volt for full-scale deflection, because of the R108-R109 divider.

3-6. CONVERTER

a. All AC measurements are made by first converting the AC input to a DC voltage. The converter provides a maximum DC output of 5 volts for a maximum AC input of 5V RMS. In the 5 VAC position, then, range switch sections S102A and S102B couple the converter amplifier input directly to the binding posts. In the 50 VAC and 500 VAC positions, input attenuators reduce the unknown AC to provide a maximum of 5 VAC input to the first converter amplifier.

b. Three stages of amplification are employed in the converter, terminated at cathode follower V404. From the cathode, full-wave negative feedback returns to the grid of the first amplifier. Half-wave rectification and filtering of the cathode follower output result in a DC voltage that is proportional to the RMS value of the AC input up to 5 V DC.

c. The over-all frequency response of the converter is essentially flat from 30 CPS to 10 KC.

3-7. CONVERTER POWER SUPPLY

a. Plate and DC filament voltages for the converter are developed in the converter power supply. V301 and C301 provide unregulated DC to the plate of V302, the series regulator for the 250 V DC plate voltage. Differential amplifiers V303 and V304 correct the grid potential of V302 as necessary to maintain the output at 250 V DC. V305 is the series regulator for the 140 V DC converter plate supply, and is driven by differential amplifier V306 to maintain a constant output.

b. The DC filament voltage is developed in a transistorized regulator circuit consisting of TR1, TR301, and TR302. The base of TR302 is maintained at a fixed negative potential by V309, a voltage regulator. Since the filament voltage is negative, a decrease in the absolute value of this voltage will cause the emitter and collector of TR302 to become more positive. This change is amplified by TR301, and the base of TR1 is driven in a negative direction, causing more filament current to be drawn through TR1. This will return the filament voltage to its proper negative value.

c. The same half-wave power supply (CR9 and C310) that develops a negative voltage for base bias of TR302 is used to light the decimal and null multiplier lamps.

SECTION IV
MAINTENANCE

4-1. GENERAL

Maintenance of the Model 803 is seldom required. Preventive maintenance consists only of keeping the interior and exterior of the instrument clean as discussed in paragraph 4-2. A troubleshooting chart, component location diagram, tube voltage chart, and a discussion of troubleshooting is provided in paragraph 4-3. Paragraph 4-4 outlines the equipment and procedures necessary to calibrate the 803.

4-2. PREVENTIVE MAINTENANCE

a. The 803 is extremely sensitive to the slightest amount of electrical leakage from the VTVM channel to the 0 volt buss, particularly from the input grid (pin 2) of V204. This leakage becomes evident when the voltage dials are set to a high voltage with the NULL switch in any null range, and no input at the binding posts. Less than 1/4 small scale division of leakage should be indicated on the meter. Accumulations of dust and foreign matter will cause internal leakage, and should be removed as often as necessary, depending on environmental operating conditions. Most accumulations can be removed by blowing the instrument out with low pressure, clean, dry air. In older configurations of the 803, two plexiglass strips were used to insulate the VTVM printed circuit board from the metal chassis. Pay particular attention to these strips when cleaning.

b. After blowing the instrument out, clean the NULL and RANGE switches with a brush dipped in Metriclene Solvent M-4, manufactured by the John B. Moore Corp., Nutley, New Jersey. In older instruments, also clean the above mentioned plexiglass strips with this solvent. After cleaning the switches, recoat the ceramic surfaces of the switches with a 10% solution of Dow Corning 200 Fluid (100 viscosity grade) in Metriclene. This prevents moisture from collecting across the ceramic surfaces.

c. When cleaning the binding post, insulators and front panel, do not use Metriclene Solvent. Use only denatured alcohol and a clean cloth, as the insulator material is slightly soluable in Metriclene.

d. If necessary, lubricate the detent mechanisms and shaft bearings of the switches sparingly. In no case should lubricant be applied to switch wafers, as leakage will result.

4-3. TROUBLESHOOTING

a. Failure of the 803 to operate properly is usually traced to failure or aging of one or more of the tubes to the point where they can no longer operate satisfactorily in the circuit. The schematic diagram and the circuit description in Section III should be reviewed before attempting to troubleshoot the instrument. The schematic is layed out in a functional manner with left-to-right signal flow in general.

b. When it becomes necessary to replace one or more tubes, it must be realized that certain tubes in the 803 perform critical functions, and replacements must be selected. Such tubes are the following:

(1) V8 is a high-mu dual triode, type 12AX7, used as a differential amplifier. Some replacement tubes may have poor balance between halves causing poor regulation against line voltage in the 500 V DC reference supply. Check for this by allowing 5 minutes for tube to heat and then varying line voltage from 105 to 130 volts and checking reference supply output voltage with another Model 803 or 801. The 500 volts must not change by more than 50 millivolts (0.01%) over this range of line voltage. If regulation exceeds this figure, discard tube in favor of another. Such discards may work very well for V206 in the chopper amplifier since it is an AC coupled amplifier not dependent upon the DC tube characteristics for proper performance.

(2) V204 is a medium-mu dual triode used in a cathode follower type VTVM circuit. The two requirements of V204 for satisfactory performance are good balance between halves and low grid current. These can be checked by setting RANGE switch to 500 V DC, NULL switch to 1V and all five voltage knobs to zero. Allow a few minutes for tube heating and then check for ability to zero meter. At zero, the VTVM-10V-1V zero knob pointer should lie within $\pm 90^{\circ}$ of vertical. If outside these limits remove tube and try another. If okay, vary line voltage from 105 to 130 VAC and check stability of meter zero. Meter should not offset more than ±4%. (2 small scale divisions). If excessive offset exists, check the heater voltage to determine whether the 9-7 ballast tube is functioning properly. Heater voltage at 117 VAC line should measure between 5.5 and 6.5 volts and should change less than 0.5 volt for a line voltage change from 105 to 130 volts. If outside these limits,

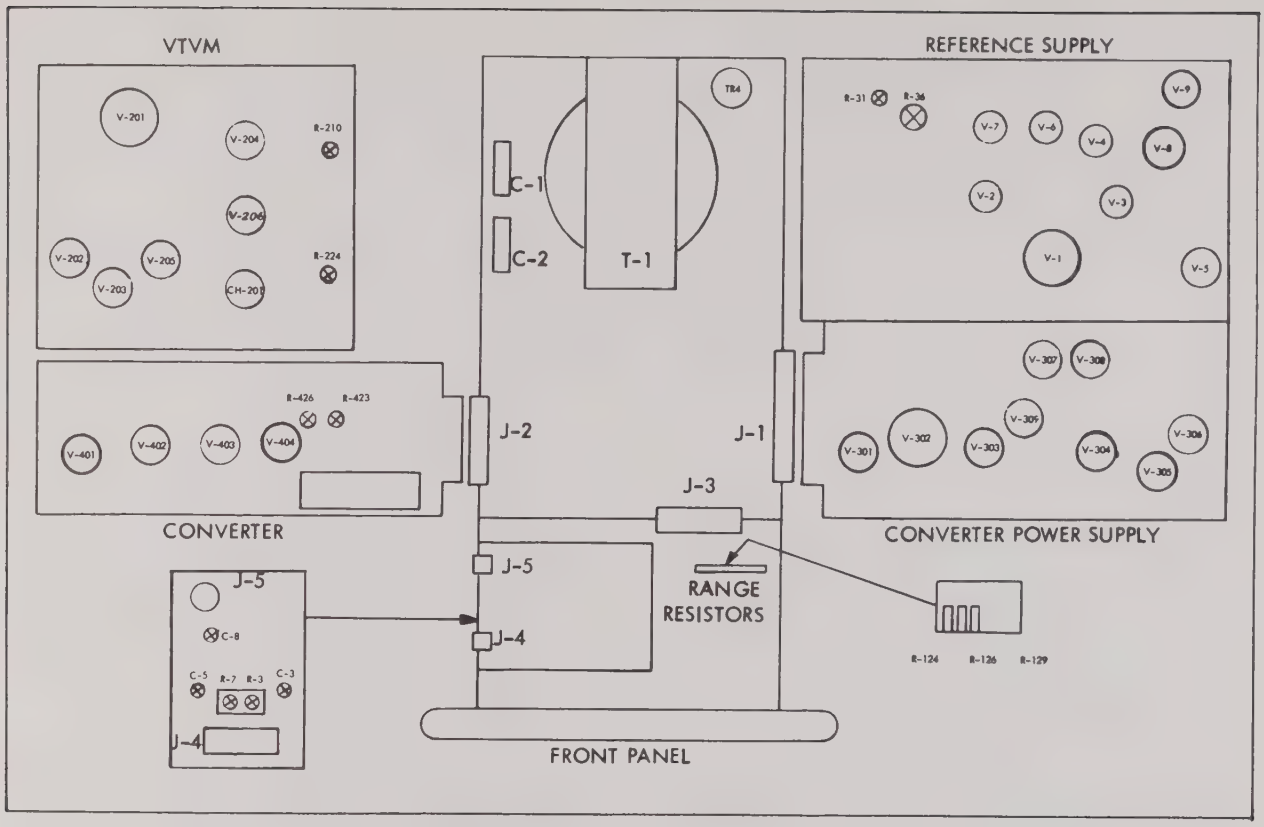

Figure 4-1. COMPONENT LOCATION

replace the 9-7. If the ballast tube is functioning properly but the meter offset exceeds 2 small scale divisions for a 25 volt change in line voltage, discard V204 in favor of another tube with better balance. To check for excessive grid current in V204, set RANGE switch to 500 V DC, NULL switch to 1V, the five voltage knobs to zero, and line voltage to 117 volts. Zero meter, then short the input binding posts. Meter offset must not exceed 1/4 of one small scale division; if it does, replace V204.

(3) V401 is a sharp cutoff pentode used as the first stage of the converter three stage feedback amplifier. It is important that this tube not be microphonic to prevent meter rattle when measuring AC voltage.

(4) Replacement of V206, the 12AX7 chopper amplifier tube should be made with one which is not microphonic. The Westinghouse type 12DF7 is a low microphonic version of the 12AX7 and may be used if desired. A microphonic or otherwise noisy tube may cause meter rattle in the 0.01 and 0.1 volt null ranges. Another possible source of meter rattle in these ranges is a defective OB2 (V203).

c. Figure 4-1 is a component location diagram showing the location of all tubes. Figure 4-2 gives the pin voltage of all tubes as an aid to troubleshooting. Figure 4-3 is a troubleshooting chart that documents the cause and remedies for the most common symptoms of instrument malfunction.

d. The standard cell of the 803 deserves special consideration if it is suspected of being faulty:

(1) The standard cell used in the Model 803 is an Eppley type MIN 1. This is a miniature low hysteresis unit which has excellent long term stability and negligible temperature hysteresis. (Hysteresis is a temporary increase in EMF immediately following a decrease in temperature; this effect should not be confused with temperature coefficient). Under normal conditions this cell should last from 8 to 15 years. In rare instances, failure has occurred in less than 2 years. End of life is usually marked by an increase in temperature hysteresis effect. That is, reading errors in excess of 0.05% will result when the same voltage is read with the 803 hot and cold. Should replacement of the cell become necessary for any reason, the instrument must be recalibrated (basic 500 volt range only), since the EMF of different cells may be different by as much as 0.05% and each instrument is calibrated to its own particular standard cell. Refer to the recalibration instructions in this case.

(2) Failure of the standard cell may occur if subjected to below freezing temperature. The electrolyte will freeze at -17°C and operation below 0°C is definitely not recommended. The life of the cell also will be greater if the 803 is not operated at elevated temperatures. The 8 to 15 year figure holds for operation of the instrument in normal room temperature.

(3) The EMF of the standard cell will change if the cell has been inverted, or if the cell has been inadvertantly short-circuited. If the EMF has changed, the 803 will naturally be out of calibration on all ranges. In either case, the cell will return to its original EMF. If the cell were inverted or shorted for only a few seconds, the 803 should be able to measure voltages within specifications after several hours recovery time.

TUBE VOLTAGE CHART*

Symbol & Type	Pin 1	Pin 2	Pin 3	Pin 4	Pin 5	Pin 6	Pin 7	Pin 8	Pin 9
V1, 5Y3GT	0	1000	0	a-c 800	0	a-c 800	0	1000	-
V2, 6AQ5A	620	660	660	660	1000	1000	630	-	-
V3, 6AU6	146	150	150	150	630	280	150	-	-
V4, OA2	150	0	0	0	150	0	0	-	-
V5, 12AU7	660	420	500	500	500	500	400	420	500
V6, OG3	170	85	170	0	170	22	85	-	-
V7, OG3	85	0	85	0	85	3.6	0	-	-
V8, 12AX7	420	170	170	170	170	410	170	170	170
V9, 9-7	0	170	0	0	0	0	170	-	-
V201, 9-7	108	0	0	0	0	108	0	-	--
V202, OA2	150	0	0	0	150	0	0	-	-
V203, OB2	108	0	0	0	108	0	0	0	-
V204, 12AU7	108	0	6	a-c 6.3	a-c 6.3	108	0	6	a-c 6.3
V205, 6C4	101	0	a-c 6.3	a-c 6.3	100	0	6.3	-	-
V206, 12AX7	85	-.71	.15	a-c 6.3	a-c 6.3	82	-1.13	0	a-c 6.3
V301, 6X4	a-c 380	a-c 380	260	260	260	a-c 380	460	-	-
V302, 5881	260	260	460	460	245	255	255	255	-
V303, 6AW8	180	175	260	a-c 6.3	a-c 6.3	180	175	260	245
V304, 12AX7	175	86	87	0	0	175	85	87	0
V305, 6AQ5A	130	140	0	0	260	260	143	-	-
V306, 6AW8	44	42	140	a-c 6.3	a-c 6.3	44	38.5	140	143
V307, OG3	85	0	85	0	85	7.5	0	-	-
V308, OA2	0	-150	0	-150	0	0	-150	-	-
V309, OG3	0	-85	0	-85	0	-6.2	-85	-	-
V401, 6DK6	0	1.75	0	-6.4	106	134	0	-	-
V402, 6DK6	0	1.65	0	-6.4	98	134	0	-	-
V403, 6DK6	0	2.5	0	-6.4	150	145	0	-	-
V404, 12AU7	260	150	150	-6.8	-6.8	260	140	142	0

*This chart is to be used under the following conditions: (a) range switch set to 500 V DC; (b) null switch set to VTVM; (c) line voltage at 117 V, 60 cycles; (d) all measurements made from negative binding post to specified terminal; (e) all measurements made with a VTVM; (f) all voltage dials set to zero; and (g) zero adjust pots counter-clockwise..

Figure 4-2. TUBE VOLTAGE CHART

e. The mercury cell, B201, is used as a source of grid bias voltage in the chopper-amplifier. This cell has an expected life in the instrument from 2 to 4 years. Replacement should be made when the cell voltage falls below 1.2 volts. A defective cell usually is evidenced by inability to zero the 0.1V-0.01V null ranges.

f. The chopper, G1, normally has a life approaching that of the standard cell. However, if the contacts are overloaded often or for extended periods of time, the contacts become corroded and the chopper-amplifier will not work properly. Poor chopper operation is indicated by erratic needle movements in the 0.1V and 0.01V null ranges, or reduced sensitivity in these ranges.

4-4. CALIBRATION

a. GENERAL. Calibration of the Model 803 should be accomplished in a draft-free area with an ambient temperature of 72°F ±5°F for maximum accuracy under typical laboratory operating conditions. DC calibration must be performed prior to AC calibration and consists of: setting the gain of the VTVM circuit; setting chopper-amplifier gain; calibrating the 500 V DC reference supply; and calibrating the 50, 5, and 0.5 V DC range dividers of the reference supply. AC calibration consists of calibrating the converter on the basic 5 VAC range, and calibrating the converter input attenuator in the 50 VAC and 500 VAC ranges. See figure 4-1 for adjustment locations.

b. DC CALIBRATION (See figure 4-4).

(1) Place instrument in operation and allow at least one hour warm-up time.

(2) Set up the necessary equipment to provide DC voltages of 500, 50, 5, and 0.5 V DC with an accuracy of at least 0.01%. The recommended equipment and method of connection is shown in figure 4-4. The required voltages are obtained by: setting the standard cell voltage on the ESI divider; putting 500 V DC into the divider from a Model 301C or 301E power supply; and zeroing the galvanometer when the push button switches are pressed by means of the vernier control on the power supply (ESI divider set at 500V). 500, 50, 5, and 0.5 V DC ±0.01% are available at the output posts of the divider by merely changing positions of the right hand knob.

(3) Place the RANGE switch in the 0.5.V DC position, and the NULL switch to VTVM.

(4) Zero the meter with the VTVM-10V-1V zero control.

(5) Apply 0.5 V DC to the instrument, and adjust R210 for full scale meter deflection. This calibrates the VTVM circuit.

(6) Remove the 0.5 V DC input.

(7) Set all voltage dials to zero and place a 39K resistor across the input terminals.

(8) Set RANGE switch to 5 V DC, and NULL switch to the 0.01V null range.

(9) Zero the meter with the 0.1V-0.01V zero control.

(10) Turn C voltage dial to 1.

(11) Using an insulated screwdriver, adjust R224 for exactly one small scale division less than left full scale meter deflection. This calibrates the chopper-amplifier gain.

(12) Begin calibration of the 500 V DC reference supply by setting voltage dials to 499.910, RANGE switch 500 V-DC, and NULL switch to 1V range.

(13) Adjust VTVM-10V-1V control for zero meter deflection.

(14) Apply 500 V DC ±0.01% to instrument.

(15) Turn ADJ CAL potentiometer for zero meter deflection. If knob is not centered approximately, turn knob to center position, remove instrument from case, and adjust R31 for zero meter deflection.

(16) Turn OFF-ON-CAL switch (OPERATE-CAL on rack models) to the CAL REF position.

(17) Adjust 0.1V-0.01V zero control for zero meter deflection.

(18) Advance OFF-ON-CAL switch to the CAL ADJ position, and adjust R36 for zero meter deflection.

(19) Return OFF-ON-CAL switch to the ON position. Meter should still read zero. If not, repeat from step (12).

(20) Remove 500 V DC input.

(21) Place RANGE switch in 50 V DC position, NULL switch to 0.1V range, and leave voltage dials at 49.9910.

(22) Adjust 0.1V-0.01V control for zero meter deflection.

(23) Apply 50 V DC ±0.01% to instrument.

(24) Adjust 50 V DC range potentiometer R124 for zero meter deflection.

(25) Remove 50 V DC input, set RANGE switch to 5 V-DC, NULL switch to the 0.01V range, and leave voltage dials at 4.99910.

(26) Apply 5 V DC ±0.01% to instrument.

(27) Adjust 5 V DC range potentiometer R126 for zero meter deflection.

(28) Remove 5 V DC input, set RANGE switch to 0.5 V DC, leave NULL switch at 0.01V range, and voltage dials at .499910.

(29) Apply 0.5 V DC ±0.01% to instrument.

(30) Adjust 0.5 V DC range potentiometer R129 for zero meter deflection.

(31) Remove 0.5 V DC input. This completes DC calibration.

c. AC CALIBRATION. Calibration of the Model 803 has been accomplished at frequencies of 400 cycles and 10 kilocycles since serial number 2625. Prior to that instrument, calibration frequencies were 400 cycles and 5 kilocycles. The AC calibration equipment recommended herein is capable of producing calibrating voltages of 500, 50, and 5 VAC ±0.05% at frequencies of 400 cycles and 10 kilocycles, with less than 0.1% total harmonic distortion. Instruments with lower serial numbers than 2625 should be calibrated at 5 KC with this same equipment, with the exception of the Elin oscillator. Elin Model VC-555 will provide 5 KC.

(1) After DC calibration has been completed, set up the equipment as shown in figure 4-5. The required AC voltages are obtained by: Setting up a precise DC voltage with the power supply-differential voltmeter combination that has the same value as the AC voltage required; the precise DC voltage is then compared with the oscillator AC voltage at the Model 540A transfer device, and the oscillator output is adjusted so that the RMS value of the oscillator output is exactly the same as the precise DC voltage.

(2) Calibrate the basic 5 VAC range by setting the voltage dials to zero, RANGE switch to 5 V DC and NULL switch to 0.01V range.

(3) Adjust 0.1V-0.01V zero control for zero meter deflection.

(4) Place NULL switch to VTVM and RANGE switch to 5 VAC.

SYMPTOM	PROBABLE CAUSE	REMEDY
Drift of the 500 V DC reference supply evidenced by the continual need for resetting the 500 V DC with the ADJ CAL potentiometer	V6, V7, or V8 defective.	Check by replacement V6, V7, and V8.
	One of the sampling string resistors R30, R32, R33, R34, and R35) is changing value rapidly as the instrument warms up.	Locate faulty resistor by heating slightly with a soldering iron held near the resistor while observing the 500 V DC calibration.
	Drifting standard cell EMF possibly caused by previous shorting or inverting of the cell.	Allow time for the standard cell to stabilize. Several hours should be sufficient.
Cannot calibrate 500 V DC reference supply. Meter cannot be brought to zero before ADJ CAL knob reaches limit.	Excessive aging of V6 or V7.	Check by replacement V6 and V7.
	Out of calibration.	Recalibrate per paragraph 4-4.
	One or more resistors in 500 V DC sampling string has shifted in value.	Recalibrate per paragraph 4-4 and observe stability for 48 hours. If 500 V DC reference supply remains stable, replacement of resistor is unnecessary.
	Standard cell EMF has shifted.	Recalibrate instrument and observe stability of reference supply. Replacement of the standard cell may be necessary.
Measurements are out of tolerance on one DC range other than the 500 V DC range.	A range resistor in the reference supply output is out of tolerance.	If the trouble occurs in the 50 V DC range, R123 has shifted; in the 5 V DC range, R125 or R127 has shifted; in 0.5 V DC range, R128 or R130 has shifted. It may be possible to correct by recalibration. If not, replace faulty resistor.
Measurements are out of tolerance on all DC ranges other than the 500 V DC range.	R120 or R121 has shifted in value.	It may be possible to correct all range voltages by recalibration. If not, replace faulty resistor.
Measurements are out of tolerance on any range when the Kelvin-Varley divider is dialed to any setting other than 499910.	One of the Kelvin-Varley divider resistors is out of tolerance	Measure the voltage drop across each Kelvin-Varley resistor with another John Fluke Differential Voltmeter. Begin by setting RANGE switch to 500 V DC and the voltage dials to 499.910. Reference to the schematic diagram will show that there should be 100, 10, 1, 0.1, and 0.01 volts respectively across each resistor of the A, B, C, D, and E decades, except for the two resistors of each decade that are paralled by the following decade. Across these two resistors, there should be 50, 5, 0.5, and 0.05 volts, respectively. Measure all voltages ±0.05%. Remember that if one resistor in a decade has increased or decreased appreciably, the voltage drop across all other resistors in the decade will be slightly affected also.

Figure 4-3. TROUBLESHOOTING (Sheet 1 of 3)

SYMPTOM	PROBABLE CAUSE	REMEDY
VTVM drift is observed by the need for frequent readjustment of the VTVM-10V-1V zero control.	V203, V204, or V202 are faulty.	Check tubes by replacement in the order specified.
Instrument out of specifications on all ranges except 0.5 V DC when used as a VTVM.	Resistor R116, R114, R112 or R110 out of tolerance.	Check and replace faulty resistor.
Meter rattle, drift, or error is observed in the 0.1V or 0.01V null ranges with or without a voltage applied.	V206 faulty.	Replace V206.
	Mercury cell B201 faulty.	Replace B201.
	V205 faulty.	Replace V205.
	Chopper G1 faulty.	Replace chopper.
	NOTE: After any of the above components are replaced, recalibration of the chopper-amplifier gain is necessary. See paragraph 4-4.	
Meter needle offsets to left as voltage dials are increased with NULL switch in the 1V null range, RANGE switch at 500 V DC and no input applied.	Leakage between the VTVM circuit and to 0 volt buss.	Clean instrument as outlined in paragraph 4-2, a.
	If instrument has not been used for a long period of time, leakage may be due to accumulation of moisture.	Leave instrument on for several hours to dry out.
NOTE: The following symptoms are common to AC measurements only, and assume all DC measurements are normal.		
Instrument out of specifications on either 500 VAC or 50 VAC range.	500 VAC or 50 VAC range out of calibration.	Perform AC calibration. If necessary, substitute new converter input attenuator components for the suspected range.
Instrument out of specifications on all AC ranges.	Input voltage is being loaded by capacitor C101.	Reverse input leads.
	V401, V402, V403, or V404 defective.	Check by replacement.
AC readings are in error only at specific frequencies.	SC401 or SC402 defective.	Replace SC401 and/or SC402.

Figure 4-3. TROUBLESHOOTING (Sheet 2 of 3)

SYMPTOM	PROBABLE CAUSE	REMEDY
Meter rattle, particularly in the 5 VAC range and 0.01V null position.	DC filament voltage on V401 thru V404 too high, caused by defective transistor TR1 or TR302 in converter power supply.	Check by replacement TR1 and TR302. (Make certain the collector of TR1 does not short to the chassis via the mounting bracket) If the tubes have operated with a filament voltage in excess of 7 V-DC, it is necessary to replace V401, and usually V402 through V404.
	Poor electrical contact between the converter and converter power supply printed circuit boards and their respective connectors.	Check printed circuit board connectors.
	Leaky cathode by-pass capacitor on V401, V402, or V403	Check and replace faulty capacitor.

Figure 4-3. TROUBLESHOOTING (Sheet 3 of 3)

(5) Short input posts and turn NULL switch to 0.01V.

(6) Adjust R426 for zero meter deflection. A long time constant in this circuit makes this a slow adjustment.

(7) Turn NULL switch to VTVM, remove the short from the input posts, and set voltage dials to 499910.

(8) Apply 5 VAC at 400 cycles to the input posts.

(9) Turn NULL switch to 0.01V and adjust the meter to read between 0.2 and 0.4 on the right side of the lower meter scale by adjusting R423.

(10) Turn NULL switch to VTVM.

(11) Change 5 VAC 400 cycle input to 5 VAC 10 KC input.

(12) Turn NULL switch to 0.01V and adjust C8 to indicate same meter deflection as step 9.

(13) Turn NULL switch to VTVM and RANGE switch to 50 VAC.

(14) Change input to 50 VAC, 400 cycles.

(15) Turn NULL switch to 0.01V and using an insulated screwdriver, adjust R3 to indicate same meter deflection as step(9).

(16) Turn NULL switch to VTVM.

(17) Change 50 VAC 400 cycle input to 50 VAC 10 KC input.

(18) Turn NULL switch to 0.01V and adjust C3 with an insulated screwdriver to indicate same meter deflection as step (9).

(19) Turn NULL switch to VTVM and RANGE switch to 500 VAC.

(20). Change input to 500 VAC, 400 cycles.

(21) Turn NULL switch to 0.01V and adjust R7 with an insulated screwdriver to indicate same meter deflection as step (9).

(22) Turn NULL switch to VTVM.

(23) Change 500 VAC 400 cycle input to 500 VAC 10 KC input.

(24) Turn NULL switch to 0.01V and adjust C5 with an insulated screwdriver to indicate same meter deflection as step (9).

(25) Return the NULL switch to the VTVM position. The AC section of the instrument is now calibrated.

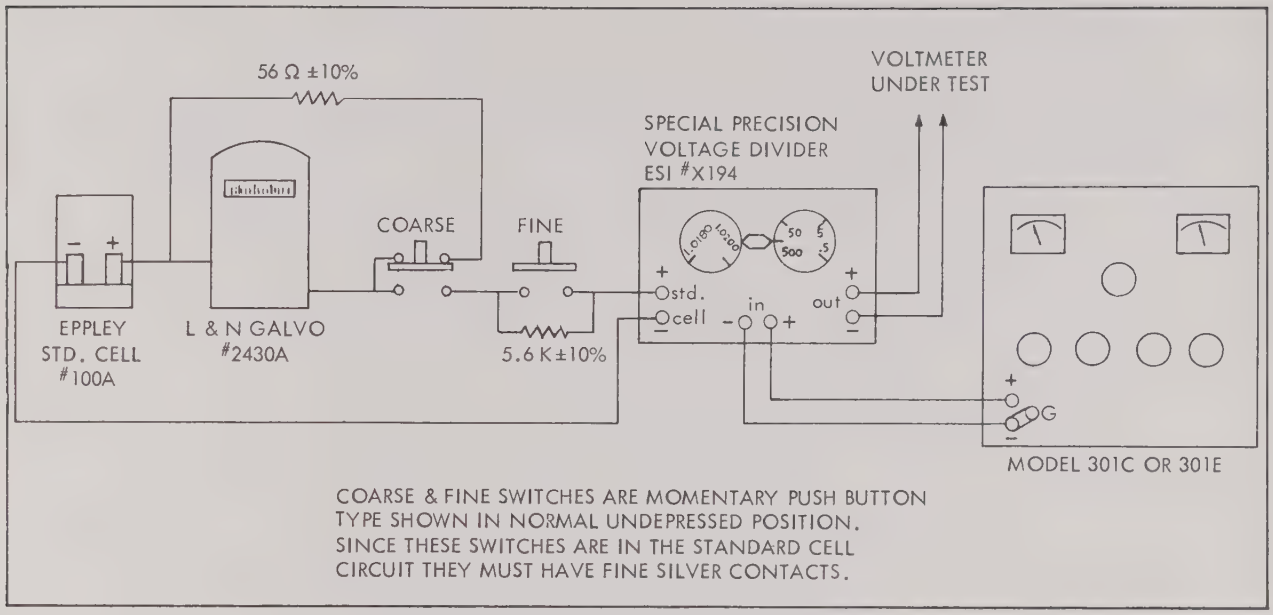

Figure 4-4. DC CALIBRATION SET-UP

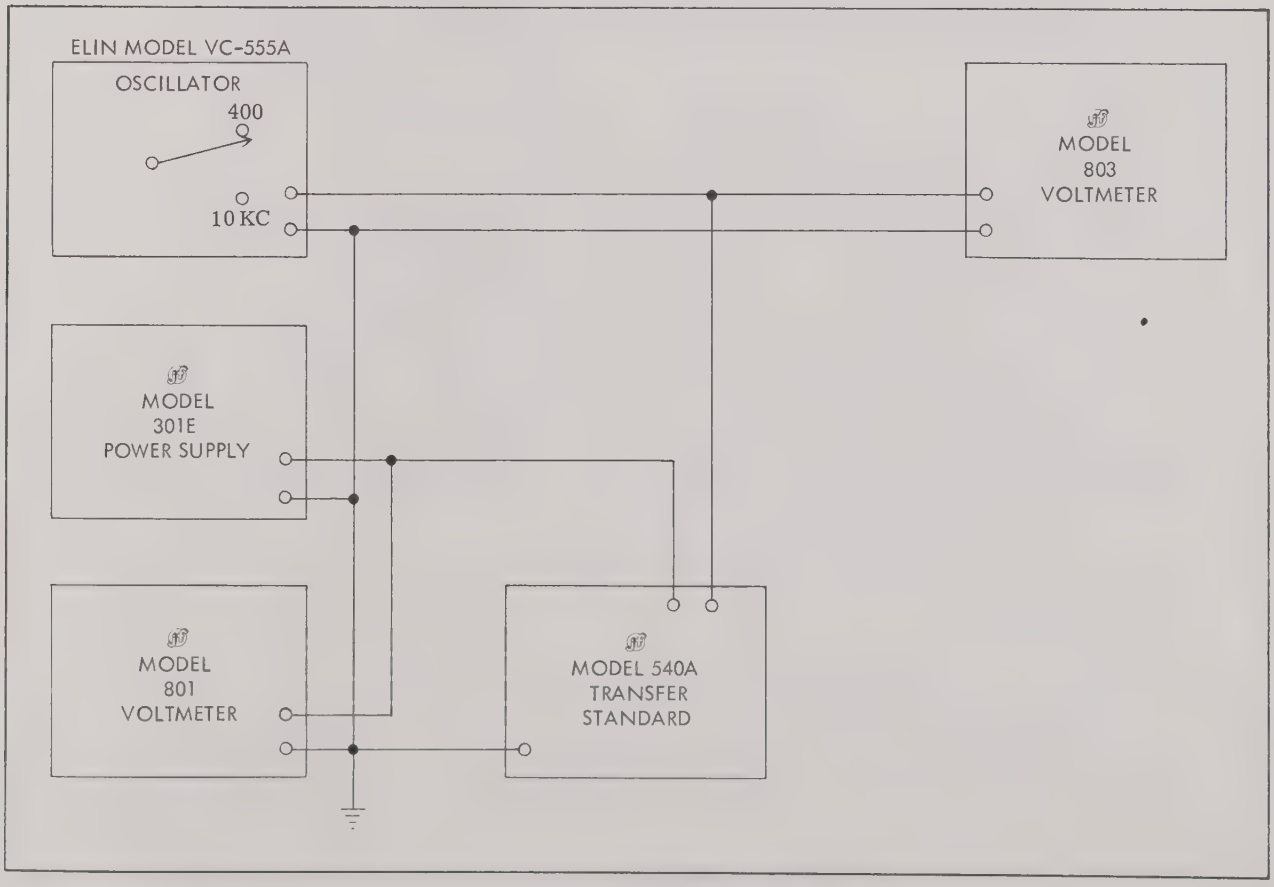

Figure 4-5. AC CALIBRATION SET-UP

SECTION V
LIST OF REPLACEABLE PARTS

The following list of replaceable parts covers all Model 803 voltmeters above serial number 1113 and all Model 803R voltmeters above serial number 406.

The extreme right hand column of the parts list, entitled "Use Code," defines the effectivity of the particular part. A list of all "Use Codes" and their effectivity is included at the end of this section.

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
B1	Standard cell, non-saturated, low hysteresis	X223	
B201	Mercury bias cell, 1.35 V	X44	
C1, C2	Capacitor, oil, 1 mfd, 1000V	CO20	D
C1A, C1B, C1C	Capacitor, electrolytic, 20 mfd, 450V	CE65	E
C3, C5	Capacitor, ceramic, variable, 0.8 - 4.5 mmf	CA4	
C6	Capacitor, ceramic, 300 mmf, 600V	CT13	
C7	Capacitor, mylar, 0.47 mfd, 600V	CP21	
C8	Capacitor, ceramic, variable, 0.8 - 4.5 mmf	CA4	
C9	Capacitor, ceramic, 20 mmf, 600V	CT14	
C10	Capacitor, paper, 0.1 mfd, 600V	CP5	
C11	Capacitor, paper, 0.1 mfd, 400V	CP4A	
C12	Capacitor, paper, 0.01 mfd, 1600V	CP1	
C13	Capacitor, ceramic, 0.002 mfd, 1000V	CT8	
C14	Capacitor, paper, 0.1 mfd, 600V	CP5	
C101	Capacitor, mylar, 1 mfd, 600V	CP33	
C102	Capacitor, polystyrene, 1 mfd, 200V	CO22	
C103	Capacitor, metalized mylar, 0.47 mfd, 600V	CP25	
C104	Capacitor, electrolytic, 200 mfd, 6V DC	CE30	A
C105	Capacitor, mylar, 0.1 mfd, 600V	CP20	A
C201, C202	Capacitor, electrolytic, 10/10 mfd, 500V	CE20	
C203	Capacitor, mylar, 0.02 mfd, 600V	CP18	
C204, C205, C206, C207	Capacitor, paper, 0.047 mfd, 400V	CP6	

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
C208	Capacitor, paper, 220 mmf, 600V	CT1	
C209	Capacitor, paper, 0.047 mfd, 400V	CP6	
C210	Capacitor, paper, 0.01 mfd, 600V	CP7	
C211, C212	Capacitor, mylar, 0.22 mfd, 400V	CP19	
C301	Capacitor, electrolytic, 10/10 mfd, 500V	CE20	
C302	Capacitor, paper, 0.1 mfd, 400V	CP4A	
C303	Capacitor, paper, 0.047 mfd, 400V	CP6A	
C304	Capacitor, electrolytic, 10/10 mfd, 500V	CE20	
C305	Capacitor, paper, 0.1 mfd, 400V	CP4A	
C306	Capacitor, fixed paper, 0.1 mfd, 400V	CP4A	
C307	Capacitor, electrolytic, 8 mfd, 250V	CE10	
C307	Capacitor, electrolytic, 8 mfd, 450V	CE77	I
C308	Capacitor, electrolytic, 4000 mfd, 15V	CE23	
C309	Capacitor, fixed paper, 0.1 mfd, 400V	CP4A	
C310	Capacitor, electrolytic, 8 mfd, 250V	CE10	
C310	Capacitor, electrolytic, 8 mfd, 450V	CE77	I
C311	Capacitor, paper, 220 mmf, 600V	CT1	
C401	Capacitor, electrolytic, 150 mfd, 150V	CE22	
C402	Capacitor, paper, 0.01 mfd, 400V	CP16	
C403	Capacitor, electrolytic, 100 mfd, 6V	CE21	
C404	Capacitor, paper, 0.47 mfd, 200V	CP24	
C405	Capacitor, paper, 0.047 mfd, 400V	CP6A	
C406	Capacitor, electrolytic, 150 mfd, 150V	CE22	
C407	Capacitor, paper, 0.01 mfd, 400V	CP16	
C408	Capacitor, electrolytic, 100 mfd, 6V	CE21	
C409	Capacitor, paper, 0.01 mfd, 400V	CP16	
C410	Capacitor, paper, 0.47 mfd, 200V	CP24	
C411	Capacitor, paper, 0.01 mfd, 400V	CP16	
C413	Capacitor, electrolytic, 100 mfd, 6V	CE21	
C414	Capacitor, ceramic, 680 mmf, 600V	CT3	
C415	Capacitor, mylar, 5 mfd, 200V	CP22	
C416	Capacitor, metalized paper, 2 mfd, 200V	CP14	
C417	Capacitor, metalized paper, 1 mfd, 200V	CP17	

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
CR1, CR2	Diode, silicon, 50V, 1 Amp.	RE8	
CR3, CR4	Diode, silicon, 280V RMS, 0.3 Amp.	2E4	
CR5, CR6	Diode, silicon, 600 PIV, 0.75 Amp.	RE17	
CR7, CR8	Diode, silicon, 40V, 2 ma	RE7	
CR9	Diode, silicon, 600 PIV, 0.75 Amp.	RE17	
F1	Fuse, 3 Amp.	F3	
F1	Fuse, 1.5 Amp (for 220/234 volt operation)	F1.5	
F101	Fuse, 1/200 Amp. 250V	F1/200A	A
G1	Chopper, SPDT, 6.3V, 60 cycles	X100	
I-103 thru I-108	Lamp, neon, NE2E	X40B	
J101	Binding post, red insulators	X219, X217	
J102	Binding post, black insulators	X219, X218	
J103	Binding post, metal spacer	X219, X220	
M101	Meter, 50-0-50 microamp with special scale	M31A	
R1	Resistor, precision metal film 1 Meg. 1%, 1/2W	DRMF71	
R2	Resistor, precision metal film 122 K, 1%, 1/2W	DRMF61	
R3	Resistor, wirewound, variable 5 K, 10%, 1/4W	P5000TA	
R4, R5	Resistor, precision metal film 500 K, 1%, 1/2W	DRMF63	
R6	Resistor, precision metal film 10 K, 1%, 1/2W	DRMF79	
R7	Resistor, wirewound, variable 500 Ω, 10%, 1/4W	P500T	
R8	Resistor, precision metal film 1 Meg. 1%, 1/2W	DRMF71	
R9	Resistor, precision metal film 200 K, 1%, 1/2W	DRMF62	
R10	Resistor, composition 390 Ω, 10%, 1W	GB3911	
R11	Resistor, composition 470 K, 10%, 1/2W	EB4741	

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
R126	Resistor, wirewound, variable 500 Ω, 10%, 1/4W	P500T	
R127	Resistor, precision wirewound 22.5 K, 0.1%, 1/2W	PR513	
R128	Resistor, precision wirewound 250.31 Ω, 0.05%, 1/2W	PR311	
R129	Resistor, wirewound, variable 500 Ω, 10%, 1/4W	P500T	
R130	Resistor, precision wirewound 24.75 K, 0.1%, 1/2W	PR514	
*R131 thru R136	Resistor, precision wirewound 40 K, 0.02%, 1/2W, matched	PR512	
*R137 thru R147	Resistor, precision wirewound 8 K, 0.05%, 1/2W, matched	PR48	
*R148 thru R158	Resistor, precision wirewound 1.6 K, 0.1%, 1/2W, matched	PR46	
*R159 thru R169	Resistor, precision wirewound 320 Ω, 0.1%, 1/2 W, matched	PR39	
*R170 thru R179	Resistor, precision wirewound 64 Ω, 0.1%, 1/2W, matched	146167	
R180, R181	Resistor, composition 150 K, 10%, 1/2W	EB1541	
R182	Resistor, composition 1 K, 10%, 1W	GB1021	
R183	Resistor, variable 300 Ω, 10%, 2W	P300A	AB
R201, R202	Resistor, composition 56 Ω, 10%, 1W	GB5601	
R203., R204	Resistor, composition 2.7 K, 10%, 1W	GB2721	
R205 thru R209	Resistor, composition 4.7 K, 10%, 1W	GB4721	
R210	Resistor, wirewound, variable 5 K, 10%, 2W	P5KA	
R211, R212	Resistor, deposited carbon 8.2 K, 1%, 1/2W	DR411	
R213, R214	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R215	Resistor, composition 10 K, 10%, 1W	GB1031	
R216, R217	Resistor, composition 39 K, 10%, 1W	GB3931	

*These resistors are factory matched for each instrument. When ordering, specify instrument serial number for each resistor ordered.

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
R218	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R219	Resistor, composition 2.2 Meg. 10%, 1/2W	EB2251	
R220	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R221	Resistor, deposited carbon 2.2 Meg. 1%, 1/2W	DR73	
R222	Resistor, composition 10 Meg. 10%, 1/2W	EB1061	
R223	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R224	Resistor, wirewound, variable 10 K, 10%, 2W	P10KA	
R225	Resistor, deposited carbon 5 K, 1%, 1/2W	DR49	
R226, R227	Resistor, composition 220 K, 10%, 1/2W	EB2241	
R228	Resistor, composition 2.2 Meg. 10%, 1/2W	EB2251	
R303	Resistor, composition 150 K, 10%, 1/2W	EB1541	
R304	Resistor, composition 220 K, 10%, 1/2W	EB2241	
R305	Resistor, composition 150 K, 10%, 1/2W	EB1541	
R306	Resistor, deposited carbon 250 K, 1%, 1W	DR613	
R307	Resistor, deposited carbon 125 K, 1%, 1/2W	DR629	
R308	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R309, R310	Resistor, composition 680 K, 10%, 1/2W	EB6841	
R311	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R312	Resistor, deposited carbon 45 K, 1%, 1W	DR58	
R313	Resistor, deposited carbon 90 K, 1%, 1/2W	DR513	
R314	Resistor, composition 470 K, 10%, 1/2W	EB4741	

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
R315	Resistor composition 100 K, 10%, 1/2W	EB1041	
R316	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R317	Resistor, deposited carbon 100 K, 1%, 1/2W	DR61	
R318	Resistor, deposited carbon 40 K, 1%, 1W	DR57	
R319	Resistor, deposited carbon 90 K, 1%, 1/2W	DR513	
R320, R321	Resistor, composition 150 K, 10%, 1/2W	EB1541	
R322	Resistor, deposited carbon 3.89 K, 1%, 1/2W	DR414	
R323	Resistor, deposited carbon 50 K, 1%, 1/2W	DR59	
R324, R325	Resistor, composition 10 K, 10%, 1W	GB1031	
R326	Resistor, composition 15 K, 10%, 1W	GB1531	
R327	Resistor, wirewound 7.5 Ω, 5%, 5W	R7.5W	
R328	Resistor, composition 10 K, 10%, 1/2W	EB1031	A
R401	Resistor, composition 3.3 K, 10%, 1W	GB3321	
R402	Resistor, composition 1.5 K, 10%, 1W	GB1521	
R403	Resistor, composition 220 Ω, 10%, 1/2W	EB2211	
R404, R405	Resistor, composition 2.2 Meg. 10%, 1/2W	EB2251	
R406	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R407, R408	Resistor, composition 3.3 K, 10%, 1W	GB3321	
R409	Resistor, composition 220 Ω, 10%, 1/2W	EB2211	
R410, R411	Resistor, composition 10 Meg. 10%, 1/2W	EB1061	
R412	Resistor, composition 360 Ω, 5%, 1W	GB3615	

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
R413	Resistor, composition 1 Meg. 10%, 1/2W	EB1051	
R414	Resistor, composition 27 K, 10%, 1W	GB2731	
R415	Resistor, composition 560 Ω, 10%, 1/2W	EB5611	
R416	Resistor, composition 100Ω, 10%, 1/2W	EB1011	
R417 thru R419	Resistor, composition 33 K, 10%, 1W	GB3331	
R420, R421	Resistor, precision metal film 22 K, 1%, 1/2W	DRMF52	
R422	Resistor, precision metal film 2.4 K, 1%, 1/2W	DRMF42	
R423	Resistor, wirewound, variable 100 Ω, 10%, 1/4W	P100T	
R424, R425	Resistor, deposited carbon 50 K, 1%, 1/2W	DR59	
R426	Resistor, wirewound, variable 5 K, 10%, 1/4W	P5000T	
R427	Resistor, composition 220 Ω, 10%, 1/2W	EB2211	
R428, R429	Resistor, composition 10 Ω, 10%, 1W	GB1001	
R430	Resistor, composition 1 K, 10%, 1W	GB1021	
S101	Switch, rotary, 3 pole, 4 position Cabinet Model 803 Rack Model 803	 803-808 803R-804	
S102	Switch, rotary, 10 pole, 7 position	SR39	
S103	Switch, rotary, 6 pole, 5 position	SR29	
S104	Switch, rotary, 2 pole, 5 position	SR40	
S105, S106 S107	Switch, rotary, 2 pole, 10 position	SR41	
S108	Switch, rotary, 2 pole, 11 position	SR42	
S109	Switch, toggle (rack model only)	ST1	
T1	Transformer assembly, harnessed Cabinet Model 803 Rack Model 803	 803-611 803R-611	
TR1	Transistor, power	2N285A	D
TR1	Transistor, power	2N301W	E

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
TR301, TR302	Transistor, NPN junction	2N214	
V1	Vacuum tube Rectifier, 5AR4	5AR4	C
V1	Vacuum tube rectifier, 5Y3GT	5Y3GT	B
V2	Vacuum tube pentode, 6AQ5A	6AQ5A	
V3	Vacuum tube pentode, 6AU6	6AU6	
V4	Vacuum tube voltage regulator, OA2	OA2	
V5	Vacuum tube duo triode, 12AU7	12AU7	
V6, V7	Vacuum tube voltage reference, OG3	OG3	
V8	Vacuum tube duo triode, 12AX7	12AX7	
V9, V201	Vacuum tube current regulator, 9-7	9-7	
V202	Vacuum tube voltage regulator, OA2	OA2	
V203	Vacuum tube voltage regulator, OB2	OB2	
V204	Vacuum tube duo triode, 12AU7	12AU7	
V205	Vacuum tube triode, 6C4	6C4	
V206	Vacuum tube duo triode, 12AX7	12AX7	
V301	Vacuum tube rectifier, 6X4	6X4	
V302	Vacuum tube beam power, 5881	5881	
V303	Vacuum tube triode-pentode, 6AW8	6AW8	
V304	Vacuum tube duo triode, 12AX7	12AX7	
V305	Vacuum tube pentode, 6AQ5A	6AQ5A	
V306	Vacuum tube triode-pentode, 6AW8	6AW8	
V307	Vacuum tube voltage reference, OG3	OG3	
V308	Vacuum tube voltage regulator, OA2	OA2	
V309	Vacuum tube voltage reference, OG3	OG3	
V310	Lamp, neon, NE83	170167	
V401, V402, V403	Vacuum tube pentode, 6DK6	6DK6	
V404	Vacuum tube duo triode, 12AU7	12AU7	
	Connector, 18 pin female	X150	
	Connector, 10 pin female	X151	
	Connector, 24 pin female	X254	
	Connector, 9 pin male	X149	

CIRCUIT SYMBOL	DESCRIPTION	FLUKE STOCK NO.	USE CODE
	Connector, 4 pin female	X177	
	Connector, 24 pin male	X255	
	Connector, 9 pin female	X153	
	Connector, 4 pin male	X178	
	Cord, power	X27D	
	Feet, rubber mounting	X224	
	Fuse holder	X12	
	Knob, 1-1/2" with pointer	X234	
	Knob, 1-1/2" without pointer	X207	
	Knob, 1" with pointer	X231	

USE CODE EFFECTIVITY

The following list of "Use Codes" is intended to allow the customer to determine the effectivity of all replaceable parts. Note that those parts with no code are used on all 803 voltmeters above serial number 1113, and all 803R voltmeters above serial number 406.

USE CODE	EFFECTIVITY
No Code	Model 803 serial number 1113 and on Model 803R serial number 406 and on
A	Model 803 serial number 1488 and on Model 803R serial number 610 and on
B	Model 803 serial number 1113 thru 1500 Model 803R serial number 610 thru 745
C	Model 803 serial number 1500 and on Model 803R serial number 610 and on
D	Model 803 serial number 1113 thru 2110 Model 803R serial number 610 thru 835
E	Model 803 serial number 2110 and on Model 803R serial number 835 and on
F	Model 803 serial number 1113 thru 2170 Model 803R serial number 610 thru 845
G	Model 803 serial number 2170 and on Model 803R serial number 845 and on
H	Model 803 serial number 1113 thru 2244 Model 803R serial number 610 thru 875
I	Model 803 serial number 3150 and on Model 803R serial number 1136 and on

Appendix A

Federal Supply Code for Manufacturers

A-1. CODE TO NAME

A-2. The following five-digit code numbers are listed in numerical sequence along with the manufacturer's name and address to which the code has been assigned. The Federal Supply Code has been taken from Cataloging Handbook H 4-2, Code to Name.

00213 Sage Electronics Corp.
Rochester, New York

00327 Welwyn International, Inc.
Westlake, Ohio

00656 Aerovox Corp.
New Bedford, Massachusetts

00779 AMP Inc.
Harrisberg, Pennsylvania

01121 Allen-Bradley Co.
Milwaukee, Wisconsin

01281 TRW Semiconductors
Lawndale, California

01295 Texas Instruments, Inc.
Semiconductor Components Div.
Dallas, Texas

01686 RCL Electronics Inc.
Manchester, New Hampshire

01730 Deleted

01884 Dearborn Electronics Inc.
Orlando, Florida

02114 Ferroxcube Corp.
Saugerties, New York

02606 Replaced by 15801

02660 Amphenol-Borg Elect. Corp.
Broadview, Illinois

02799 Arco Capacitors, Inc.
Los Angeles, California

03614 Replaced by 71400

03651 Replaced by 44655

03797 Eldema Corp.
Compton, California

03877 Transitron Electronic Corp.
Wakefield, Massachusetts

03888 Pyrofilm Resistor Co., Inc.
Cedar Knolls, New Jersey

03911 Clairex Corp.
New York, New York

03980 Muirhead Instruments, Inc.
Mountainside, New Jersey

04009 Arrow Hart and Hegemen
Electronic Company
Hartford, Connecticut

04062 Replaced by 72136

04202 Replaced by 81312

04217 Essex Wire Corp
Wire & Cable Div.
Anaheim, California

04221 Aemco
Div. of Midtex Inc.
Mankato, Minnesota

04645 Replaced by 75376

04713 Motorola Semiconductor
Products Inc.
Phoenix, Arizona

05082 Replaced by 94154

05236 Jonathan Mfg. Co.
Fullerton, California

05277 Westinghouse Electric Corp.
Semiconductor Dept.
Youngwood, Pennsylvania

05278 Replaced by 43543

05397 Union Carbide Corp.
Electronics Div.
Cleveland, Ohio

05571 Sprague Electric Co
Pacific Div.
Los Angeles, California

05704 Alac, Inc.
Glendale, California

05820 Wakefield Engineering Ind.
Wakefield, Massachusetts

06001 General Electric Company
Capacitor Department
Irmo, South Carolina

06136 Replaced by 63743

06473 Amphenol Space & Missile Sys.
Chatsworth, California

06555 Beede Electrical Instrument Co.
Penacook, New Hampshire

06739 Electron Corp.
Littletown, Colorado

06743 Clevite Corp.
Cleveland, Ohio

06751 Semcor Div. Components
Phoenix, Arizona

06860 Gould National Batteries Inc.
City of Industry, California

06980 Eitel-McCullough, Inc.
San Carlos, California

07115 Replaced by 14674

07138 Westinghouse Electric Corp
Electronic Tube Div.
Elmira, New York

07263 Fairchild Semiconductor
Div. of Fairchild Camera
& Instrument Corp.
Mountain View, California

07344 Bircher Co., Inc.
Rochester, New York

07792 Lerma Engineering Corp
Northampton, Massachusetts

07910 Continental Device Corp.
Hawthorne, California

08530 Reliance Mica Corp.
Brooklyn, New York

08792 CBS Electronics Semiconductor
Operations-Div. of CBS Inc.
Lowell, Massachusetts

08806 General Electric Co.
Miniature Lamp Dept.
Cleveland, Ohio

08863 Nylomatic Corp.
Norrisville, Pennsylvania

09069 Skottie Electronics Inc.
Archbald, Pennsylvania

09922 Burndy Corp.
Norwalk, Connecticut

11237 Chicago Telephone of Calif. Inc.
South Pasadena, California

11358 CBS Electronics
Div. of CBS Inc.
Newburyport, Massachusetts

11403 Best Products Co.
Chicago, Illinois

11503 Keystone Mfg
Div. of Avis Industrial Corp.
Warren, Michigan

12014 Chicago Rivet & Machine Co.
Bellwood, Illinois

12040 National Semiconductor Corp.
Danburry, Connecticut

12060 Diodes, Inc.
Chatsworth, California

12136 Philadelphia Handle Co.
Camden, New Jersey

12323 Presin Co., Inc.
Shelton, Connecticut

12327 Freeway Washer & Stamping Co.
Cleveland, Ohio

12400 Replaced by 75042

12617 Hamlin Inc.
Lake Mills, Wisconsin

12697 Clarostat Mfg. Co.
Dover, New Hampshire

12749 James Electronics
Chicago, Illinois

12856 Micrometals
Sierra Madre, California

12954 Dickson Electronics Corp.
Scottsdale, Arizona

13606 Sprague Electric Co.
Transistor Div.
Concord, New Hampshire

13839 Replaced by 23732

14099 Semtech Corp.
Newbury Park, California

14193 California Resistor Corp.
Santa Monica, California

14296 American Components, Inc.
Conshohocken, Pennsylvania

14655 Cornell-Dubilier Electronics
Newark, New Jersey

14674 Corning Glass Works
Corning, New York

14752 Electro Cube Inc.
San Gabriel, California

14869 Replaced by 96853

15636 Elec-Trol Inc.
Northridge, California

15801 Fenwal Electronics Inc.
Framingham, Massachusetts

15818 Amelco Semiconductor
Div. of Teledyne Inc.
Mountain View, California

15849 Useco, Inc.
Mt. Vernon, New York

15909 Replaced by 17870

16332 Replaced by 28478

16473 Cambridge Scientific Ind. Inc.
Cambridge, Maryland

16742 Paramount Plastics
Downey, California

16758 Delco Radio
Div. of General Motors
Kokomo, Indiana

17069 Circuit Structures Lab.
Upland, California

17856 Siliconix, Inc.
Sunnyvale, California

17870 Daven-Div. of Thomas A. Edison
Ind. --McGraw-Edison Co.
Manchester, New Hampshire

18083 Deleted

18178 Vactec Inc.
Maryland Heights, Missouri

18736 Voltronics Corp.
Hanover, New Jersey

19429 Montronics, Inc.
Seattle, Washington

19451 Perine Machinery & Supply Co.
Seattle, Washington

19701 Electra Mfg. Co.
Independence, Kansas

20584 Enochs Mfg. Co.
Indianapolis, Indiana

22767 ITT Semiconductors
Div. of ITT
Palo Alto, California

23732 Tracor
Rockville, Maryland

24248 Southco
Div. of South Chester Corp.
Lester, Pennsylvania

24655 General Radio Co.
West Concord, Massachusetts

25403 Amperex Electronic Corp
Semiconductor & Receiving
Tube Division
Slatersville, Rhode Island

28478 Deltrol Controls Corp.
Milwaukee, Wisconsin

28520 Heyman Mfg. Co.
Kenilworth, New Jersey

30323 Illinois Tool Works Inc.
Chicago, Illinois

33173 General Electric Co.
Tube Dept.
Owensboro, Kentucky

37942 Mallory, P. R., & Co., Inc.
Indianapolis, Indiana

38315 Honeywell Inc.
Precision Meter Div.
Manchester, New Hampshire

42498 National Company
Melrose, Massachusetts

43543 Nytronics Inc.
Transformer Co. Div.
Alpha, New Jersey

44655 Ohmite Mfg. Co.
Skokie, Illinois

49671 Radio Corp. of America
New York, New York

49956 Raytheon Company
Lexington, Maine

53021 Sangamo Electric Co.
Springfield, Illinois

55026 Simpson Electric Company
Chicago, Illinois

56289 Sprague Electric Co.
North Adams, Massachusetts

58474 Superior Electric Co.
Bristol, Connecticut

60399 Torrington Mfg. Co.
Torrington, Connecticut

62460 Deleted

63743 Ward Leonard Electric Co.
Mount Vernon, New York

64834 West Mfg. Co.
San Francisco, California

65092 Weston Instruments Inc.
Newark, New Jersey

66150 Winslow Tele-Tronics Inc.
Asbury Park, New Jersey

70563 Amperite Company
Union City, New Jersey

70903 Belden Mfg. Co.
Chicago, Illinois

71002 Birnbach Radio Co., Inc.
New York, New York

71400 Bussmann Mfg.
Div. of McGraw-Edison Co.
St. Louis, Missouri

71450 CTS Corp.
Elkhart, Indiana

71468 ITT Cannon Electric Inc.
Los Angeles, California

71482 Clare, C P. & Co.
Chicago, Illinois

71590 Centralab
Div. of Globe Union Inc.
Milwaukee, Wisconsin

71707 Coto Coil Co., Inc.
Providence, Rhode Island

71744 Chicago Miniature Lamp Works
Chicago, Illinois

71785 Cinch Mfg. Co. & Howard
B. Jones Div.
Chicago, Illinois

72005 Driver, Wilber B., Co.
Newark, New Jersey

72092 Replaced by 06980

72136 Electro Motive Mfg. Co.
Willimantic, Connecticut

72259 Nytronics Inc.
Berkeley Heights, New Jersey

72354 Deleted

72619 Dialight Corp
Brooklyn, New York

72653 G. C. Electronics
Rockford, Illinois

72665 Replaced by 90303

72794 Dzus Fastener Co., Inc.
West Islip, New York

72928 Gudeman Co.
Chicago, Illinois

72982 Erie Tech. Products Inc.
Erie, Pennsylvania

73138 Beckman Instruments Inc.
Helipot Division
Fullerton, California

73293 Hughes Aircraft Co.
Electron Dynamics Div.
Newport Beach, California

73445 Amperex Electronic Corp.
Hicksville, New York

73559 Carling Electric Inc.
Hartford, Connecticut

73586 Circle F Industries
Trenton, New Jersey

73734 Federal Screw Products, Inc.
Chicago, Illinois

73743 Fischer Special Mfg. Co.
Cincinnati, Ohio

73899 JFD Electronics Co.
Brooklyn, New York

73949 Guardian Electric Mfg. Co.
Chicago, Illinois

74199 Quam Nichols Co.
Chicago, Illinois

74217 Radio Switch Corp.
Marlboro, New Jersey

74276 Signalite Inc.
Neptune, New Jersey

74306 Piezo Crystal Co.
Carlisle, Pennsylvania

74542 Hoyt Elect. Instr. Works
Penacook, New Hampshire

74970 Johnson, E. F., Co.
Waseca, Minnesota

75042 IRC Inc.
Philadelphia, Pennsylvania

75376 Kurz-Kasch, Inc.
Dayton, Ohio

75382 Kulka Electric Corp.
Mt. Vernon, New York

75915 Littlefuse Inc.
Des Plaines, Illinois

76854 Oak Mfg. Co.
Crystal Lake, Illinois

77342 Potter & Brumfield
Div. of Amer. Machine & Foundry
Princeton, Indiana

77969 Rubbercraft Corp. of Calif. LTD.
Torrance, California

78189 Shakeproof
Div. of Illinois Tool Works
Elgin, Illinois

78277 Sigma Instruments, Inc.
South Braintree, Massachusetts

78488 Stackpole Carbon Co.
St. Marys, Pennsylvania

78553 Tinnerman Products
Cleveland, Ohio

79136 Waldes Kohinoor Inc.
Long Island City, New York

79497 Western Rubber Company
Goshen, Indiana

79963 Zierick Mfg. Corp.
New Rochelle, New York

80031 Mepco
Div. of Sessions Clock Co.
Morristown, New Jersey

80145 API Instruments Co.
Chesterland, Ohio

80183 Sprague Products
North Adams, Massachusetts

80294 Bourns Inc.
Riverside, California

80583 Hammarlund Co., Inc.
Mars Hill, North Carolina

80640 Stevens, Arnold Inc.
Boston, Massachusetts

81073 Grayhill Inc.
La Grange, Illinois

81312 Winchester Electronics
Div. of Litton Industries
Oakville, Connecticut

81439 Therm-O-Disc Inc.
Mansfield, Ohio

81483 International Rectifier Corp.
El Segundo, California

81590 Korry Mfg Co.
Seattle, Washington

82376 Deleted

82389 Switchcraft Inc.
Chicago, Illinois

82415 Price Electric Corp.
Frederick, Maryland

82872 Roanwell Corp.
New York, New York

82877 Rotron Mfg. Co., Inc.
Woodstock, New York

82879 ITT Wire & Cable Div.
Pawtucket, Rhode Island

83003 Varo Inc.
Garland, Texas

83298 Bendix Corp.
Electric Power Division
Eatontown, New Jersey

83330 Smith, Herman H., Inc.
Brooklyn, New York

83478 Rubbercraft Corp. of America
New Haven, Connecticut

83594 Burroughs Corp.
Electronic Components Div.
Plainfield, New Jersey

83740 Union Carbide Corp.
Consumer Products Div.
New York, New York

84171 Arco Electronics, Inc.
Great Neck, New York

84411 TRW
Ogallala, Nebraska

86577 Precision Metal Products
Stoneham, Massachusetts

86684 Radio Corp. of America
Electronic Components &
Devices
Harrison, New Jersey

86689 Deleted

87034 Marco-Oak Inc.
Anaheim, California

88419 Use 14655

88690 Replaced by 04217

89536 Fluke, John Mfg. Co., Inc.
Seattle, Washington

89730 Replaced by 08806

90201 Mallory Capacitor Co.
Indianapolis, Indiana

90215 Best Stamp & Mfg. Co.
Kansas City, Missouri

90211 Square D Co.
Chicago, Illinois

90303 Mallory Battery Co.
Tarrytown, New York

91293 Johanson Mfg. Co.
Boonton, New Jersey

91407 Replaced by 58474

91637 Dale Electronics Inc.
Columbus, Nebraska

91662 Elco Corp.
Willow Grove, Pennsylvania

91737 Gremar Mfg. Co., Inc.
Wakefield, Massachusetts

91802 Industrial Devices, Inc.
Edgewater, New Jersey

91836 King's Electronics
Tuckahoe, New York

91929 Honeywell Inc.
Micro Switch Div.
Freeport, Illinois

91934 Miller Electric Co., Inc.
Pawtucket, Rhode Island

93332 Sylvania Electric Products
Semiconductor Products Div.
Woburn, Massachusetts

94145 Replaced by 49956

94154 Tung-Sol
Div. of Wagner Electric Corp.
Newark, New Jersey

95146 Alco Electronics Products Inc.
Lawrence, Massachusetts

95263 Leecraft Mfg. Co.
Long Island City, New York

95264 Replaced by 98278

95275 Vitramon Inc.
Bridgeport, Connecticut

95303 Radio Corp. of America
Solid State & Receiving Tube Div.
Cincinnati, Ohio

95354 Methode Mfg. Corp.
Rolling Meadows, Illinois

95712 Dage Electric Co., Inc.
Franklin, Indiana

95987 Weckesser Co., Inc.
Chicago, Illinois

96733 San Fernando Electric Mfg. Co.
San Fernando, California

96853 Rustrak Instrument Co.
Manchester, New Hampshire

96881 Thomson Industries, Inc.
Manhasset, New York

97540 Master Mobile Mounts
Div. of Whitehall Electronics Corp.
Los Angeles, California

97913 Industrial Electronic Hdware Corp.
New York, New York

97945 White, S. S. Co.
Plastics Div.
New York, New York

97966 Replaced by 11358

98094 Replaced by 49956

98278 Microdot Inc.
Pasadena, California

98291 Sealectro Corp.
Conhex Div
Mamaroneck, New York

98388 Accurate Rubber & Plastics
Culver City, California

98743 Replaced by 12749

98925 Deleted

99120 Plastic Capacitors, Inc.
Chicago, Illinois

99217 Southern Electronics Corp.
Burbank, California

99515 Marshall Industries
Capacitor Div.
Monrovia, California

Revised August 1, 1968
Using H4-1 and H4-2
Dated June, 1968

Appendix C

Sales Representatives & Service Centers

ALABAMA

HUNTSVILLE
BCS Associates, Inc.
2317 Bob Wallace Ave.
P.O. Box 1273
Tel. (205) 881-6220
Zip 35807

ALASKA

SEATTLE
Showalter-Judd, Inc.
1806 S. Bush Place
Seattle, Washington 98144
Tel. (206) 324-7911

ARIZONA

*PHOENIX
Barnhill Associates
537 E. Osborn Road, Suite 4
Tel. (602) 263-1250
Zip 85012

CALIFORNIA

***LOS ANGELES
Instrument Specialists, Inc.
1109 S. Central Ave.
Glendale, California 91204
Tel (213) 245-9404

**SANTA CLARA
Instrument Specialists, Inc.
2359 De La Cruz Blvd.
Tel. (408) 244-1505
Zip 95050

SAN DIEGO
Instrument Specialists, Inc.
1901 State St.
Tel. (714) 232-2017
Zip 92101

COLORADO

*DENVER
Barnhill Associates
1170 S. Sheridan Blvd.
Tel. (303) 934-5505
Zip 80226

CONNECTICUT

HARTFORD
Instrument Representatives, Inc.
P. O. Box 165
Glastonbury, Connecticut 06033
Tel (203) 633-0777

FLORIDA

**ORLANDO
BCS Associates, Inc.
940 N. Fern Creek Ave.
P.O. Box 6578
Tel. (305) 843-1510
Zip 32803

GEORGIA

ATLANTA
BCS Associates, Inc.
1230 Briar Hill Dr.
Tel. (404) 874-9925
Zip 30306

HAWAII

HONOLULU
Industrial Electronics, Inc.
646 Queen Street
P.O. Box 135
Tel. (808) 533-6095
Zip 96817

ILLINOIS

**CHICAGO
Cozzens & Cudahy, Inc.
9501 W. Devon Ave.
Rosemont, Illinois 60018
Tel. (312) 825-1144

INDIANA

INDIANAPOLIS
Cozzens & Cudahy, Inc.
Port O'Call Executive Ctr.
21 Beachway Drive
Tel. (317) 244-2456
Zip 46234

MARYLAND

**BALTIMORE
Electronic Marketing Assoc. Inc.
11501 Huff Court
Kensington, Maryland 20795
Tel. (301) 881-5300

MASSACHUSETTS

**BOSTON
Instrument Representatives, Inc.
1046 Massachusetts Avenue
Arlington, Massachusetts 02174
Tel. (617) 646-1034

MICHIGAN

DETROIT
WKM Associates, Inc.
1474 East Outer Dr.
Tel. (313) 892-2500
Zip 48234

MINNESOTA

MINNEAPOLIS
Cozzens & Cudahy, Inc.
7450 France Ave. So.
Tel. (612) 920-1022
Zip 55435

MISSOURI

ST. LOUIS
Cozzens & Cudahy, Inc.
P. O. Box 10013
Lambert Field - Zip 63145
Tel. (314) 423-1234

NEW JERSEY

**NEWARK
SBM Associates, Inc.
1519 Stuyvesant Avenue
Union, New Jersey 07083
Tel. (201) 687-8737

NEW MEXICO

*ALBUQUERQUE
Barnhill Associates
1410—D Wyoming N.E.
Tel. (505) 299-7658
Zip 87110

NEW YORK

*NEW YORK
SBM Associates, Inc.
28 Hobby Street
Pleasantville, N. Y. 10570
Tel. (914) 769-1811

**ROCHESTER
SBM Associates, Inc.
4515 Culver Rd.
Tel. (716) 266-1400
Zip 14622

NORTH CAROLINA

GREENSBORO
BCS Associates, Inc.
1039 E. Wendover Ave.
P.O. Box 6426
Tel. (919) 273-1918
Zip 27405

OHIO

*CLEVELAND
WKM Associates, Inc.
16141 Puritas Ave.
Tel. (216) 267-0445
Zip 44135

*DAYTON
WKM Associates, Inc.
6073 Far Hills Ave.
Tel. (513) 434-7500
Zip 45429

OREGON

PORTLAND
Showalter-Judd, Inc.
1445 N. E. Arrington
Hillsboro, Oregon 97123
Tel. (503) 648-6372

PENNSYLVANIA

PHILADELPHIA
Electronic Marketing Assoc.
210 Goddard Blvd.—Suite 100
King of Prussia, Pennsylvania
Tel (215) 248-5050
Zip 19406

PITTSBURGH
WKM Associates, Inc.
90 Clairton Blvd.
Tel. (412) 892-2953
Zip 15236

TEXAS

*DALLAS
Barnhill Associates
Suite 220
312 N. Central Express Wy.
Richardson, Texas 75080
Tel. (214) 231-2573

*HOUSTON
Barnhill Associates
Suite 332
3810 Westheimer
Tel. (713) 621-0040
Zip 77027

EAST VIRGINIA

WILLIAMSBURG
BCS Associates, Inc.
107 Rich Neck Road
Tel. (703) 229-5108
Zip 23185

WASHINGTON

SEATTLE
Showalter-Judd, Inc.
1806 S. Bush Place
Seattle, Washington 98144
Tel. (206) 324-7911

CANADA

BRITISH COLUMBIA

VANCOUVER
Allan Crawford Associates, Ltd.
1820 Pandora St.
Tel. (604) 253-7136

ONTARIO

*MALTON
Allan Crawford Associates, Ltd.
6427 Northam Drive.
Tel. (416) 678-1500

OTTAWA, 3
Allan Crawford Associates, Ltd.
376 Churchill Ave. — Suite 106
Tel. (613) 725-3354

QUEBEC

LONGUEUIL
Allan Crawford Associates, Ltd.
157 (rue) St. Charles Street W.
Tel. (514) 670-1212

DOMESTIC SERVICE CENTERS

*** DESIGNATES FLUKE REGIONAL SERVICE CENTER
** DESIGNATES REPRESENTATIVE OFFICES WITH SERVICE CENTERS
* DESIGNATES REPRESENTATIVE OFFICES SERVED BY AUTHORIZED CONTRACT SERVICE LABORATORIES

INTERNATIONAL REPRESENTATIVES

ARGENTINA

Coasin S.A.
Virrey del Pino 4071
Buenos Aires, Argentina

AUSTRALIA

Elmeasco Instruments
7 Chard Road
P.O. Box 324
Brookvale, N.S.W. Australia 2100

AUSTRIA

Kontron GMBH & Co., Kg.
Lederergasse 16
1080 Wien
Austria

BELGIUM

C. N. Rood S/A
37, Place de Jamblinne de Meux
B-1040 Brussels, Belgium

BRAZIL

AMBRIEX S.A.
Av. Graca Aranha
226—6º And.
Rio De Janeiro, Brazil

AMBRIEX S.A.
Av. Pacaembu, 811
Sao Paulo, Brazil

CHILE

Coasin Chile Ltd.
Casilla 14588
Correo 15
Santiago, Chile

DENMARK

Tage Olsen A/S
1, Ronnegade
Copenhagen 0, Denmark

FINLAND

Oy Findip AB
Postbox 52025
Helsinki 52, Finland

FRANCE

Radio Equipment Antares
9, Rue Ernest Cognacq
92 Levallois — Perret
France

HONG KONG

Gilman & Co. Ltd.
P.O. Box 56
Hong Kong

INDIA

Hinditron Services Pvt. Ltd.
69/A Nepean Sea Road
Bombay 6, India

ISRAEL

R.D.T. Electronics Eng'r. Ltd.
P.O. Box 21082
Tel-Aviv, Israel

ITALY

Elettronucleonica S.P.A.
7, P.zza De Angeli
20146 Milano, Italy

JAPAN

Toyo Trading Co., Ltd.
P.O. Box 5014
International Tokyo
Japan

2-38 Junkeicho-dori
Minami-ku, Osaka, Japan

KOREA

M-C International
I.P.O. Box 1355
Seoul, Korea

MALAYSIA

O'Connor's (Pte) Ltd.
P.O. Box 1197
Kota Kinabalu
East Malaysia

P.O. Box 91
Pataling Jaya
West Malaysia

MEXICO

Mexitek, S.A.
Eugenia 408
Departments 1 y 5
Mexico 12, D.F.

THE NETHERLANDS

C.N. Rood N.V.
Post Office Box 4542
Rijswijk (Z.H.) 2100
The Netherlands

Fluke (Nederland) N.V.
Post Office Box 5053
Industrieterrein Noord
Tilburg, The Netherlands

NEW ZEALAND

Elmeasco Instruments (Pty) Ltd.
P.O. Box 213
Mt. Waverley, Vic. 3149
Australia

NORWAY

Morgenstierne & Co. A/S
P.B. 6688 Rodelokka
Oslo 6, Norway

SINGAPORE

O'Connor's (Pte) Ltd.
Maybank House 124-126
Robinson Road
Singapore 1, Singapore

SOUTH AFRICA

K. Baker (Pty.) Ltd.
P.O. Box 1257
Johannesburg, So. Africa

P.O. Box 3641
Cape Town, So. Africa

P.O. Box 2143
Durban, So. Africa

SPAIN

Rema Leo Haag, S.A.
General Sanjurjo 18
Madrid 3, Spain

SWEDEN

Erik Ferner AB
Box 56
161.26 Stockholm-Bromma,
Sweden

SWITZERLAND

Kontron Electronic A.G.
Hardstrasse 235
P.O. Box 193
8031 Zurich
Switzerland

TAIWAN-REPUBLIC OF CHINA

Heighten Trading Co., Ltd.
P.O. 1408
Taipei, Taiwan, 104

THAILAND

G.Simon Radio Ltd.
30 Patpong Avenue
Suriwong
Bangkok, Thailand

THE UNITED KINGDOM

Fluke International Corp.
Garnet Close
Watford, WD2 4TT
England

URUGUAY

Coasin Uruguaya S.A.
Cerrito 617 - 4º Piso
Montevideo, Uruguay

VENEZUELA

Coasin C.A.
APDO, Postal 50939
Sabana Grande No. 1
Caracas, Venezuela

WEST GERMANY

Fey Elektronische Messgeraete
8000 Muenchen 2
Horemansstrasse 28
West Germany

In Europe, contact FLUKE NEDERLAND, N.V., POST OFFICE BOX 5053, INDUSTRIETERREIN NOORD, TILBURG, THE NETHERLANDS

FLUKE REGIONAL SERVICE CENTER; THE NETHERLANDS

FLUKE (NEDERLAND) N.V.
P. O. BOX 5053
TILBURG, THE NETHERLANDS

FLUKE REGIONAL SERVICE CENTER, UNITED KINGDOM

FLUKE INTERNATIONAL CORP.
GARNET CLOSE
WATFORD, WD2 4TT
ENGLAND

AUTHORIZED SERVICE LABORATORIES INTERNATIONAL

EACH INTERNATIONAL REPRESENTATIVE IS EQUIPPED WITH AN AUTHORIZED SERVICE LABORATORY. PLEASE REFER TO THE INTERNATIONAL REPRESENTATIVE LISTING FOR YOUR SERVICE NEEDS.

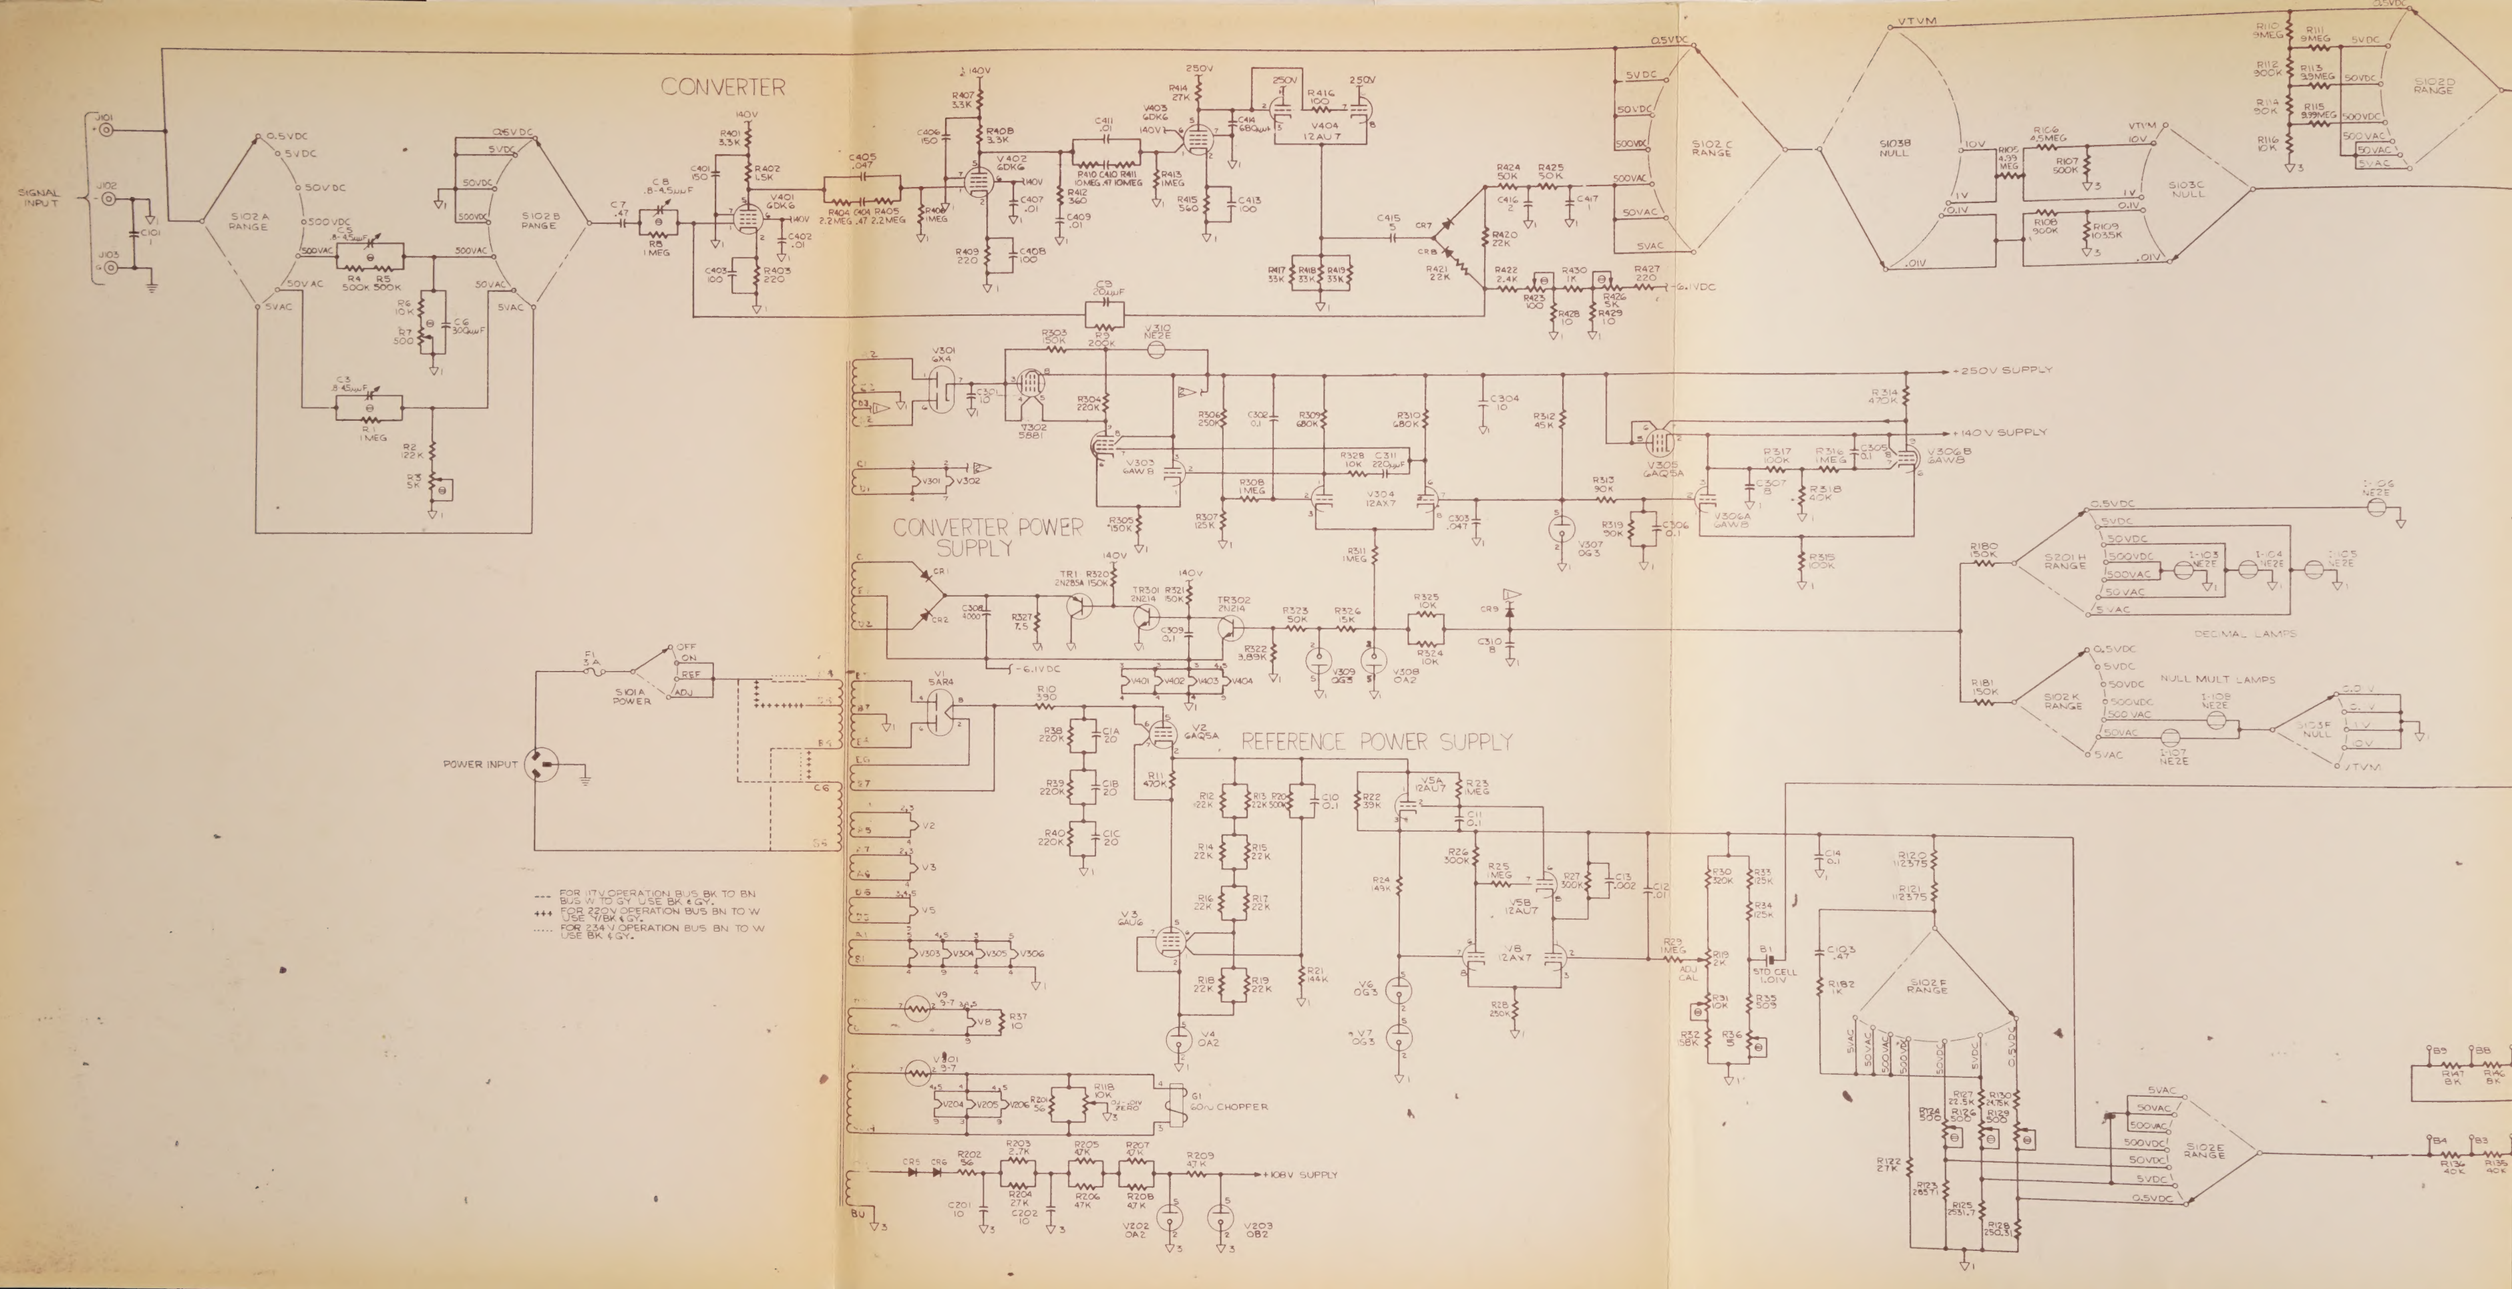
CONVERTER
CONVERTER POWER SUPPLY
REFERENCE POWER SUPPLY
SIGNAL INPUT
POWER INPUT
S102 A RANGE
S102 B RANGE
S102 C RANGE
S102D RANGE
S103B NULL
S103C NULL
S201 H RANGE
S102 K RANGE
S102 F RANGE
S102 E RANGE
S101A POWER
VTVM
DECIMAL LAMPS
NULL MULT LAMPS
STD CELL 1.01V
ADJ CAL
60~ CHOPPER
+250V SUPPLY
+140 V SUPPLY
+108V SUPPLY
--- FOR 117V OPERATION BUS BK TO BN BUS W TO GY USE BK & GY.
+++ FOR 220V OPERATION BUS BN TO W USE W/BK & GY.
..... FOR 234 V OPERATION BUS BN TO W USE BK & GY.

S103D NULL
VTVM
R104 4.5MEG
10V
1V
0.1V
.01V
OFF
ON
S101C POWER
REF
ADJ
R103 4.4M
S103E NULL
1.0V
0.1V
.01V
S101R POWER
CALIBRATE REF.
CALIBRATE ADJ.
R213 1MEG
C203 0.02
+108V
R216 39K
C205 .047
R215 10K
R220 1MEG
C206 .047
V205 6C4
R218 1MEG
R217 39K
R223 1MEG
C209 .047
V206B 12AX7
V206A 12AX7
R219 2.2MEG
C210 .01
R221 2.2MEG
C207 .047
R226 220K
R227 220K
R228 2.2MEG
R222 10 MEG
C208 220 μμf
R224 10K
C212 .22
C211 .22
R214 1MEG
C204 .047
CHOPPER-AMPLIFIER
S102G RANGE
.5VAC
5VAC
50VAC
500VAC
.5VDC
5VDC
50VDC
500VDC
R225 5K
R102 15K
B201 1.35V MERCURY CELL
60~ CHOPPER
G1
VTVM
V204A 12AU7
R212 8.2K
R117 5K
R211 8.2K
VTVM 10V-1V O ADJ
CR6
CR7
R118 500
C104 200
RECORDER OUTPUT
R210 5K
V204B 12AU7
C105 .01
F101 5MA
S108 DIAL E
S103A NULL
S101D POWER
R101 270
C102 1.0
S102J RANGE
R179 64
R178 64
R177 64
R176 64
R175 64
R174 64
R173 64
R172 64
R171 64
R170 64
S107 DIAL D
R169 320
R168 320
R167 320
R166 320
R165 320
R164 320
R163 320
R162 320
R161 320
R160 320
R155 320
S106 DIAL C
KELVIN-VARLEY DIVIDER
R158 1.6K
R157 1.6K
R156 1.6K
R155 1.6K
R154 1.6K
R153 1.6K
R152 1.6K
R151 1.6K
R150 1.6K
R149 1.6K
R148 1.6K
S105 DIAL B
R145 8K
R144 8K
R143 8K
R142 8K
R141 8K
R140 8K
R139 8K
R138 8K
R137 8K
S104 DIAL A
R134 40K
R133 40K
R132 40K
R131 40K
S104
S105
S106
S107
S108

1 = 0 VOLT BUS
3 = CHOPPER-AMP & VTVM COMMON

⊖ FOR INTERNAL ADJUSTMENT

▷ ALL FLAG NOTES WITH THE SAME NUMBER ARE CONNECTED.

803 SER. NO. 2170 & ON
803B SER. NO. 8498 ON

FUNCTIONAL SCHEMATIC
AC-DC DIFFERENTIAL VOLTMETER
MODEL 803, 803B

JOHN FLUKE MANUFACTURING COMPANY
MUKILTEO TERRACE, WASHINGTON

www.manualsplus.com
1020804